

ATOMTEX
Scientific and Production Enterprise

INSTRUMENTS AND TECHNOLOGIES FOR NUCLEAR
MEASUREMENTS AND RADIATION MONITORING

Product Catalogue

www.atomtex.com

| | |
|---|----|
| ABOUT | 3 |
| RADIATION DETECTORS (AT2522) | 4 |
| PERSONAL DOSIMETERS (AT2503B, B/1, B/2 / AT3509, A, B, C) | 5 |
| POCKET DOSIMETERS / POCKET RADIATION MONITORS (AT2140, A, A/1 / AT6130C / AT6130, A, D) | 6 |
| PORTABLE DOSIMETERS (AT1103M / AT1121, AT1123) | 7 |
| RADIATION MONITORS (AT1125, A / AT1117M) | 9 |
| WIDE-RANGE DOSIMETERS (AT2533, AT2533/1) | 15 |
| STANDARD DOSIMETERS (AT5350/1) | 16 |
| RADIONUCLIDE IDENTIFICATION DEVICES (AT1321 / AT1120M, MA / AT1120ME / AT6102, A, B) | 17 |
| FIELD SPECTROMETERS (AT6101DR) | 21 |
| IMMERSION SPECTROMETERS (AT6104DM, DM1) | 22 |
| RADIATION SCANNING EQUIPMENT (AT6101C, CE / AT6101CE / AT6103) | 23 |
| STATIONARY SPECTROMETERS AND ACTIVITY MONITORS (AT1320, A, B, C / AT1135 / AT1315 / AT1329) | 27 |
| WHOLE BODY COUNTERS (AT1316, A / AT1322, AT1322/1) | 30 |
| AREA MONITORS (AT2327, AT2331 Dosimetric systems / Area monitors for pulse radiation AT2341 Radiation Monitoring Station / Spectrometric systems) | 31 |
| PEDESTRIAN AND VEHICLE RADIATION MONITORS (AT920B, P / AT930 / AT2327 / AT6110) | 38 |
| VERIFICATION AND CALIBRATION EQUIPMENT (AT110, AT130 / AT140 / AT300 / AT200) | 45 |
| EQUIPMENT FOR NEUTRON SPECTROMETRY | 49 |
| SMART DETECTION UNITS AND DETECTION DEVICES | 50 |

About

ATOMTEX was established in 1995 and now is a leading research and manufacturing centre of the Republic of Belarus, widely recognised internationally in the area of development and production of equipment for nuclear measurements and radiation monitoring.

Highly qualified professionals with broad experience in nuclear instrumentation are at the core of our team.



Over **200** employees, including R&D, production and support staff.
The average age of staff is 45



Over **190** products



Export share **90%**



Deliveries to **127** countries of the world.
Status of permanent vendor of IAEA, CTBTO and ROSATOM.

For over 25 years our professional team bears responsibility for measurement quality of each device produced by our company as well as its functionality, usability and reliability.

Compliance of product parameters with stated performance and features is not just a slogan, but the basis of our company-to-customer relationship.



Quality management
system is certified



Member of IEC TC 45
"Nuclear Instrumentation"
from Republic of Belarus



European Nuclear Society
Corporate Member

Our high-precision and multifunctional metrological infrastructure, promotion of innovative ideas and advanced technologies, as well as orientation to international standards – all this helps us to create state-of-the-art products of high scientific and technological level.

Close cooperation with leading national, foreign and international organizations propels us in our continuous commitment to progress and improvement.

APPLICATION



Atomic Energy



Environmental
Radiation Monitoring



Robotic Systems



Industry



Homeland Security



Science and Education



Health Care



Calibration Facilities



Geophysics

AT2522 Radiation Detector (Alpha SENSOR)

Detection and quick assessment of surface contamination by alpha radionuclides, such as polonium-210.

Easy-to-operate detector can be used by persons of any skill level and in everyday life.

- Scintillation detector
- Silicon photomultiplier
- High sensitivity
- Selectable units of measurement (cps, Bq, Bq/cm²)
- Light, sound and vibration alarms
- Extended operation without recharging
- Colour 1" OLED screen



| | |
|---|---|
| Scintillation detector | ZnS(Ag), surface area 25 cm ² |
| Registration efficiency | ≥50% (α particles ²³⁹ Pu) |
| Time of continuous operation - with display ON - with display OFF | ≥40 h ≥500 h |
| Power supply | Built-in battery |
| PC connection interface and charger connector | microUSB |
| Protection class | IP40 |
| Overall dimensions, weight | 106x60x31 mm, 170 g |





AT2503B, B/1, B/2 Personal Dosimeters

Control of X-ray and gamma radiation personal dose equivalent.

The dosimeter together with the PC reader and the software forms an efficient automatic system for staff radiation exposure control.

- Simultaneous measurement of gamma radiation personal dose equivalent and personal dose equivalent rate
- Autocompensation of intrinsic detector background
- Alarm mode for detection of pulse radiation with pulse duration over 10 ns (option)

| | |
|---|--|
| Measurement range of personal dose equivalent Hp(10) | 0.1 μ Sv – 10 Sv (AT2503B, B/1) 1 μ Sv – 10 Sv (AT2503B/2) |
| Measurement range of personal dose equivalent rate Hp(10) | 0.1 μ Sv/h – 1 Sv/h (AT2503B) 0.1 μ Sv/h – 0.2 Sv/h (AT2503B/1) 1 μ Sv/h – 10 Sv/h (AT2503B/2) |
| Energy range | 50 keV – 10 MeV |
| Energy dependence relative to 662 keV (^{137}Cs) | $\pm 30\%$ |
| Response time to 10-fold dose rate change | ≤ 5 s (for dose rate value > 1 mSv/h) |
| Total run time on one set of batteries | ≥ 1000 h |
| Protection class | IP54 |
| Overall dimensions, weight | 85x46x16 mm, 70 g (w/o batteries) |



AT2503 and AT3509 Personal dosimeters meet requirements of **IEC 61526:2005** (Confirmed by IAEA-EURADOS, IAEA-TECDOC-1564 intercomparisons)

AT3509, A, B, C Personal Dosimeters

Control of X-ray and gamma radiation personal dose equivalent.

The dosimeter together with the PC reader and the software forms an efficient automatic system for staff radiation exposure control.

- Silicone planar detector
- Zero intrinsic background
- Simultaneous measurement of depth dose Hp(10) and skin dose Hp(0.07)

| Measurement | AT3509,A | AT3509B,C |
|---|---|-----------|
| Hp(10) / $\dot{\text{H}}\text{p}(10)$ | + | + |
| Hp(0.07) / $\dot{\text{H}}\text{p}(0.07)$ | – | + |
| Measurement range of personal dose equivalent Hp(10), Hp(0,07) | 1 μ Sv – 10 Sv | |
| Measurement range of personal dose equivalent rate Hp(10), Hp(0,07) | 0.1 μ Sv/h – 1 Sv/h (AT3509,A,B) 0.1 μ Sv/h – 5 Sv/h (AT3509C) | |
| Energy range | 15 keV – 10 MeV (AT3509,B,C) 30 keV – 10 MeV (AT3509A) | |
| Energy dependence relative to 662 keV (^{137}Cs) | $\pm 25\%$ (15 keV – 1.5 MeV) $\pm 60\%$ (1.5 MeV – 10 MeV) | |
| Energy dependence relative to 59.5 keV (^{241}Am) | $\pm 30\%$ (15 – 300 keV) (AT3509B,C) | |
| Response time to 10-fold dose rate change | ≤ 5 s (for dose rate value > 1 mSv/h) | |
| Total run time on one set of batteries | ≥ 500 h | |
| Protection class | IP54 | |
| Overall dimensions, weight | 105x58x23 mm, 100 g(w/o batteries) | |



Design and specifications are subject to change without notice



AT2140, A, A/1 Dosimeters

Measurement of X-ray and gamma radiation ambient dose equivalent and ambient dose equivalent rate.

- Unique combination of efficiency, response and usability
- Time of continuous operation without battery replacement (2 x AA):
AT2140 – 5000 h, AT2140A, A/1 – 10000 h
- Search mode
- USB port and software for dosimeter setup and viewing measurement results (AT2140A/1)

| | |
|--|---|
| Measurement range: - Ambient dose equivalent rate | 0.1 µSv/h – 10 mSv/h (AT2140) 0.1 µSv/h – 100 mSv/h (AT2140A, A/1) |
| - Ambient dose equivalent | 0.1 µSv – 1.99 Sv |
| Limits of tolerable intrinsic relative error | ±15% |
| Energy range | 50 keV – 3 MeV |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | ±30% (AT2140) ±25% (AT2140A, A/1) |
| Typical sensitivity to ¹³⁷ Cs gamma radiation | 1.8 cps/(µSv·h ⁻¹) |
| Response time for dose rate change from 1 to 10 µSv/h | ≤10 s (AT2140) ≤5 s (AT2140A, A/1) |
| Protection class | IP40 |
| Drop protection | ≤1.0 m height (AT2140A, A/1) |
| PC interface | USB (AT2140A/1) |
| Overall dimensions, weight | 111x70x28 mm, 110 g (w/o batteries) |



AT6130C Radiation Monitor

Measurement of X-ray and gamma radiation ambient dose equivalent and ambient dose equivalent rate.

- Robust housing from impact-resistant ABS plastic
- Convenient menu
- Search mode

| | |
|--|--------------------------------|
| Measurement range: - Ambient dose equivalent rate | 0.1 µSv/h – 1 mSv/h |
| - Ambient dose equivalent | 0.1 µSv – 100 mSv |
| Limits of tolerable intrinsic relative error | ±20% |
| Energy range | 50 keV – 3 MeV |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | ±30% |
| Typical sensitivity to ¹³⁷ Cs gamma radiation | 2.8 cps/(µSv·h ⁻¹) |
| Response time for dose rate change from 1 to 10 µSv/h | ≤7 s |
| Time of continuous operation | ≥700 h |
| Protection class | IP40 |
| Drop protection | ≤1.5 m height |
| Overall dimensions, weight | 111x70x28 mm, 0.2 kg |

Design and specifications are subject to change without notice



AT6130, A, D Radiation Monitors

Measurement of X-ray and gamma radiation ambient dose equivalent rate and ambient dose equivalent, as well as measurement of beta particle flux density (AT6130).



- Rugged metal housing
- Convenient menu
- Selective measurement of beta and gamma radiation in mixed fields (AT6130)
- Dose rate measurement up to 100 mSv/h (AT6130D)
- Search mode
- Headphones for work in noisy environments (option)

| | |
|--|--|
| Measurement range: | |
| - Ambient dose equivalent rate | 0.1 µSv/h – 10 mSv/h (AT6130,A) 0.1 µSv/h – 100 mSv/h (AT6130D) |
| - Ambient dose equivalent | 0.1 µSv – 100 mSv (AT6130,A) 0.1 µSv – 1 Sv (AT6130D) |
| Measurement range of beta particle flux density | 10 – 10 ⁴ particle·min ⁻¹ ·cm ⁻² (AT6130) |
| Limits of tolerable intrinsic relative error | ±20% |
| Energy range: | |
| - X-ray and gamma radiation | 20 keV – 3 MeV (AT6130) 50 keV – 3 MeV (AT6130A,D) |
| - Beta radiation | 155 keV – 3.5 MeV (AT6130) |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | ±30% |
| Time of continuous operation | ≥500 h |
| Protection class | IP57 |
| Drop protection | ≤1.5 m height |
| Overall dimensions, weight | 110x60x38 mm, 0.25 kg |



Gamma and beta radiation detector (AT6130)



AT1103M X-ray Radiation Dosimeter

Measurement of continuous X-ray and gamma radiation directional dose equivalent and directional dose equivalent rate.

- Unique highly-sensitive device for controlling radiation dose on the eye lens, mucous membranes and skin
- Spectrum display when connected to a PC
- Not for natural background measurement

| | |
|--|--|
| Scintillation detector | NaI(Tl), Ø9x2 mm with beryllium window |
| Measurement range: | |
| - Directional dose equivalent rate | 50 nSv/h – 100 µSv/h |
| - Directional dose equivalent | 50 nSv – 5 mSv |
| Limits of tolerable intrinsic relative error | ±15% |
| Energy range | 5 – 160 keV |
| Energy dependence relative to 59.5 keV (²⁴¹ Am) | ±35% (5 – 60 keV) ±30% (60 – 160 keV) |
| Typical sensitivity to ²⁴¹ Am gamma radiation | 400 cps/(µSv·h ⁻¹) |
| Detectable ²⁴¹ Am activity at the distance of 0.5 m in <2 s | 1000 kBq (27 µCi) |
| Protection class | IP54 |
| Overall dimensions, weight | 233x85x67 mm, 0.9 kg |



Design and specifications are subject to change without notice

AT1121, AT1123 X-ray and Gamma Radiation Dosimeters



- Measurement of continuous, short-term and pulse X-ray and gamma radiation ambient dose equivalent and ambient dose equivalent rate
- Search and detection of X-ray and gamma radiation sources
- Search and detection of high-level beta radiation sources with maximum spectrum energy of more than 500 keV
- Measurement over a wide range of dose rates and energies
- Measurement of dose rate and exposure time during short-term exposure (from 0.03 s)
- Measurement of pulse radiation average dose rate, where the pulse duration is 10 ns and longer (AT1123)
- Automatic record of over 500,000 measurement results into non-volatile memory
- One of four available averaging modes can be selected
- The remote control is available for distant measurements
- Possibility of stationary placement with external audio-visual alarm and potential-free contacts for actuator control
- Connection to a PC to form a continuous monitoring system with the documenting function



Dosimeter with remote control and alarm unit



| Detector | Scintillation tissue-equivalent plastic Ø30x15 mm |
|--|---|
| Measurement range of ambient dose equivalent rate: - Continuous radiation - Short-term radiation - Pulse radiation | 50 nSv/h – 10 Sv/h 5 µSv/h – 10 Sv/h 0.1 µSv/h – 10 Sv/h (AT1123) |
| Measurement range of ambient dose equivalent | 0.1 nSv – 100 Sv |
| Limits of tolerable intrinsic relative error | ±15% (Continuous and short-term radiation) ±30% (Pulse radiation) |
| Energy range: - Continuous and short-term radiation - Pulse radiation | 15 keV – 10 MeV 15 keV – 10 MeV (AT1123) |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | ±35% (15 – 60 keV) ±25% (60 keV – 10 MeV) |
| Typical sensitivity to ¹³⁷ Cs gamma radiation | 70 cps/(µSv·h ⁻¹) |
| Measurement time of ¹³⁷ Cs gamma radiation dose rate - Dose rate: 50 – 300 nSv/h - Dose rate: 0.3 – 2 µSv/h - Dose rate: 2 µSv/h – 10 Sv/h | ≤60 s ≤10 s ≤2 s |
| Response time for dose rate change from 0.1 to 1 µSv/h | <2 s |
| Protection class | IP54 |
| Overall dimensions, weight | 233x85x67 mm, 0.9 kg |

AT1125, AT1125A Radiation Monitors

- Measurement of X-ray and gamma radiation ambient dose equivalent and ambient dose equivalent rate
- Control of $^{137}\text{Cs}^*$ content in samples inside 0.5-liter Marinelli beaker, both with and without protection unit (PrU)
- Measurement of alpha and beta particle flux density from contaminated surfaces (external BDPS-02 detection unit**)
- Search and detection of X-ray and gamma radiation sources
- High sensitivity
- Spectrum display when connected to a PC



Activity measurement
in samples with
protection unit (1 cm lead)



Design and specifications are
subject to change without notice

| | | |
|--|------------------------------------|---|
| Detector | - AT1125 - AT1125A - BDPS-02 | Scintillation NaI(Tl) Ø25x40 mm Scintillation NaI(Tl) Ø25x40 mm and Geiger-Mueller counter tube End-type Geiger-Mueller counter tube |
| Measurement range: - Ambient dose equivalent rate - Ambient dose equivalent | | 30 nSv/h – 300 µSv/h (AT1125) 30 nSv/h – 100 mSv/h(AT1125A) 10 nSv – 10 mSv(AT1125) 10 nSv – 10 Sv(AT1125A) |
| Measurement range of ^{137}Cs specific activity | | 50 – 10^5 Bq/kg (with PrU) 100 – 10^5 Bq/kg (w/o PrU) |
| Measurement range of flux density: - Alpha particles - Beta particles | | $2.4 - 10^6$ particle·min ⁻¹ ·cm ⁻² (BDPS-02) $6 - 10^6$ particle·min ⁻¹ ·cm ⁻² (BDPS-02) |
| Limits of tolerable intrinsic relative error | | ±15% (dose rate AT1125, A) ±20% (dose rate BDPS-02) ±20% (specific activity) ±20% (flux density BDPS-02) |
| Energy range of X-ray and gamma radiation | | 50 keV – 3 MeV (AT1125, A) 20 keV – 3 MeV (BDPS-02) |
| Energy dependence relative to 662 keV (^{137}Cs) | | ±15% (AT1125,A) ±30% (BDPS-02) |
| Typical sensitivity to ^{137}Cs gamma radiation | | 350 cps/(µSv·h ⁻¹) (AT1125,A) 6.6 cps/(µSv·h ⁻¹) (BDPS-02) |
| Detectable activity of ^{137}Cs source, located at the distance of 5 cm in a time not longer than 2 s | | 10 kBq |
| Protection class | | IP54 (AT1125, A) / IP64 (BDPS-02) |
| Overall dimensions, weight | | 258x85x67 mm, 1.0 kg (AT1125,A) 138x86x60 mm, 0.3 kg (BDPS-02) Ø150x155 mm, 10.5 kg (PrU) |
| * The list of controlled radionuclides can be adjusted on request. Available variants: a) ^{137}Cs , ^{134}Cs + ^{137}Cs ; b) ^{131}I , ^{137}Cs , ^{134}Cs + ^{137}Cs | | |
| ** BDPS-02 can be substituted by the following detection units: BDPA-01, BDPA-02, BDPA-03, BDPB-01, BDPB-02 and BDPB-03. For specification of detection units see AT117M Radiation monitor (page 13) | | |

Express sample activity
measurement



0.5-liter
Marinelli
beaker

External BDPS-02
detection unit





Depending on the set of detection units (DU) the radiation monitor can be used for the measurement of:

- X-ray, gamma and neutron radiation ambient dose equivalent and ambient dose equivalent rate
- Air kerma and air kerma rate of X-ray and gamma radiation
- Directional dose equivalent and directional dose equivalent rate of continuous X-ray and gamma radiation
- Flux density of alpha and beta particles from contaminated surfaces
- Flux density and fluence of neutrons with known energy distribution
- Surface activity and disintegrations of ^{239}Pu and $^{90}\text{Sr} + ^{90}\text{Y}$
- Real-time search for sources of ionizing radiation and radioactive materials.

Operator can use either processing unit (PU/PU2/PU4) or desktop PC for operation and indication.



PU



PU2

PU4

| Processing unit | PU / PU2 | PU4 |
|---|---|---|
| Detector | Geiger-Mueller counter tube | |
| Measurement range: - Ambient dose equivalent rate - Ambient dose equivalent | 1 $\mu\text{Sv/h}$ – 100 mSv/h 1 μSv – 1 Sv | 1 $\mu\text{Sv/h}$ – 100 mSv/h 1 μSv – 100 Sv |
| Limits of tolerable intrinsic relative error | $\pm 20\%$ | |
| Energy range | 60 keV – 3 MeV | |
| Energy dependence relative to 662 keV (^{137}Cs) | -25% to +35% | |
| Typical sensitivity to ^{137}Cs gamma radiation | 1 cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | 0.33 cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) |
| Protection class | IP64 | |
| Overall dimensions | 177x85x124 mm (PU) 210x88x36 mm (PU2) | 265x90x40 mm |
| Weight | 1.2 kg (PU) / 0.6 kg (PU2) | 0.6 kg |

PU and PU2 offer the following functionality:

- Indication of dose, dose rate and count rate measurement results with statistical error value
- Manual recording, storage and transferring measurement results to a PC
- Setting threshold alarm levels

PU4 is a hand-held PC (HPC) with integrated detection module, which offers the following functionality:

- Processing and display of measurement data
- Collection of data from detection unit via Bluetooth (adapter) or cable
- GPS-referencing of measurement results
- Automatic recording and storage of large-scale measurement results
- Data import to a PC for further processing
- Automatic data transfer to a remote server (If 3G option in HPC is available)

AT1117M. X-ray and gamma radiation detection units

| | | | |
|---|--|---|---|
|  BDKG-01 | Detector | - BDKG-01 - BDKG-03 - BDKG-04 - BDKG-05 - BDKG-11 - BDKG-17 - BDKG-24 - BDKG-30 - BDKG-32 - BDKR-01 - BDPS-02 | Geiger-Mueller counter tube NaI(Tl) scintillator, Ø25x40 mm Scintillation plastic, Ø30x15 mm NaI(Tl) scintillator, Ø40x40 mm NaI(Tl) scintillator, Ø63x63 mm Geiger-Mueller counter tube Scintillation plastic, Ø50x40 mm Scintillation plastic, Ø50x40 mm Scintillation plastic, Ø70x80 mm NaI(Tl) scintillator, Ø9x2 mm Geiger-Mueller counter tube |
|  BDKG-03 | | | |
|  BDKG-04 | Measurement range of ambient radiation dose equivalent rate (Ambient dose equivalent) | - BDKG-01 - BDKG-03 - BDKG-04 - BDKG-05 - BDKG-11 - BDKG-17 - BDKG-24 - BDKG-32 - BDPS-02 | 0.1 µSv/h – 10 Sv/h (0.1 µSv – 10 Sv) 0.03 – 300 µSv/h (0.03 µSv – 1 Sv) 0.05 µSv/h – 10 Sv/h (0.7 nSv – 100 Sv) 0.03 – 300 µSv/h (0.03 µSv – 0.3 Sv) 0.03 – 100 µSv/h (0.01 µSv – 10 mSv) 1 mSv/h – 100 Sv/h (1 mSv – 100 Sv) 0.03 µSv/h – 1 Sv/h (0.1 nSv – 100 Sv) 0.03 µSv/h – 0.5 Sv/h (0.1 nSv – 100 Sv) 0.1 µSv/h – 30 mSv/h (0.1 µSv – 1 Sv) |
|  BDKG-05 | Measurement range of air kerma rate (Air kerma) | - BDKG-30 | 0.03 µGy/h – 1 Gy/h (0.1 nGy – 100 Gy) |
|  BDKG-11 | Measurement range of directional dose equivalent rate (Directional dose equivalent) | - BDKR-01 | 0.05 – 100 µSv/h (0.05 µSv – 5 mSv) |
|  BDKG-17 | Limits of tolerable intrinsic relative error | - all DUs | ±20% |
|  BDKG-24 | Energy dependence relative to 662 keV (¹³⁷ Cs) (Energy range) | - BDKG-01 - BDKG-03 - BDKG-04 - BDKG-05 - BDKG-11 - BDKG-17 - BDKG-24 - BDKG-30 - BDKG-32 - BDPS-02 | -25% to +35% (60 keV - 3 MeV) ±20% (50 keV - 3 MeV) ±25% (15 keV - 3 MeV), ±40% (3 - 10 MeV) ±20% (50 keV - 3 MeV) ±20% (50 keV - 3 MeV) -25% to +35% (60 keV - 3 MeV) ±25% (25 keV - 3 MeV), ±40% (3 - 10 MeV) ±25% (50 keV - 3 MeV), ±40% (3 - 10 MeV) ±25% (40 keV - 3 MeV), ±40% (3 - 10 MeV) ±30% (20 keV - 3 MeV) |
|  BDKG-30 | Energy dependence relative to 59.5 keV (²⁴¹ Am) (Energy range) | - BDKR-01 | ±35% (5 - 60 keV), ±30% (60 - 160 keV) |
|  BDKG-32 | Typical sensitivity to ¹³⁷ Cs gamma radiation | - BDKG-01 - BDKG-03 - BDKG-04 - BDKG-05 - BDKG-11 - BDKG-17 - BDKG-24 - BDKG-30 - BDKG-32 - BDPS-02 | 4 cps/(µSv·h ⁻¹) 350 cps/(µSv·h ⁻¹) 70 cps/(µSv·h ⁻¹) 760 cps/(µSv·h ⁻¹) 2200 cps/(µSv·h ⁻¹) 0.005 cps/(µSv·h ⁻¹) 530 cps/(µSv·h ⁻¹) 600 cps/(µSv·h ⁻¹) 1660 cps/(µSv·h ⁻¹) 6.6 cps/(µSv·h ⁻¹) |
| | Typical sensitivity to ²⁴¹ Am gamma radiation | - BDKR-01 | 400 cps/(µSv·h ⁻¹) |

Design and specifications are subject to change without notice

AT117M. X-ray and gamma radiation detection units




BDKR-01



BDPS-02

| | | |
|---|---|---|
| Response time for dose rate change from 0.1 to 1 $\mu\text{Sv/h}$ | - BDKG-03 - BDKG-04 - BDKG-05 - BDKG-11 - BDKG-24 - BDKG-32 | ≤ 2 s |
| Response time for dose rate change from 0.1 to 1 $\mu\text{Gy/h}$ | - BDKG-30 | ≤ 2 s |
| Response time for dose rate change from 1 to 10 $\mu\text{Sv/h}$ | - BDKG-01 - BDKR-01 - BDPS-02 | ≤ 3 s ≤ 2 s ≤ 3 s |
| Protection class | - all DUs | IP64 |
| Overall dimensions, weight | - BDKG-01 - BDKG-03 - BDKG-04 - BDKG-05 - BDKG-11 - BDKG-17 - BDKG-24 - BDKG-30 - BDKG-32 - BDKR-01 - BDPS-02 | $\varnothing 54 \times 256$ mm, 0.5 kg $\varnothing 60 \times 299$ mm, 0.6 kg $\varnothing 60 \times 200$ mm, 0.46 kg $\varnothing 60 \times 290$ mm, 1.2 kg $\varnothing 78 \times 320$ mm, 1.9 kg $\varnothing 54 \times 167$ mm, 0.28 kg $\varnothing 60 \times 205$ mm, 0.5 kg $\varnothing 60 \times 207$ mm, 0.6 kg $\varnothing 80 \times 245$ mm, 0.78 kg $\varnothing 60 \times 261$ mm, 0.55 kg $138 \times 86 \times 60$ mm, 0.33 kg |


AT117M. Neutron radiation detection units



BDKN-01



BDKN-03



BDKN-05

| | | |
|--|---|---|
| Detector: He-3 counter in polyethylene moderator | - BDKN-01 - BDKN-03 - BDKN-05 - BDKN-06 | one He-3 counter one He-3 counter two He-3 counters one He-3 counter |
| Measurement range of ambient dose equivalent rate [ambient dose equivalent] | - BDKN-01 - BDKN-03 - BDKN-06 | 0.1 $\mu\text{Sv/h}$ – 10 mSv/h [0.1 μSv – 10 Sv] 0.1 $\mu\text{Sv/h}$ – 10 mSv/h [0.1 μSv – 10 Sv] 0.1 $\mu\text{Sv/h}$ – 30 mSv/h [0.1 μSv – 10 Sv] |
| Measurement range of neutron flux density | - BDKN-01 - BDKN-03 - BDKN-05 | 0.1 – 10^4 $\text{neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$ 0.1 – 10^4 $\text{neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$ 0.1 – $2 \cdot 10^3$ $\text{neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$ |
| Limits of tolerable intrinsic relative error | Dose rate measurement mode Flux density measurement mode | $\pm 35\%$ $\pm 20\%$ $\pm 20\%$ $\pm 20\%$ $\pm 35\%$ $\pm 20\%$ |
| Energy range | - all DUs | 0.025 eV – 14 MeV |
| Typical sensitivity to Pu-Be radiation | Dose rate measurement mode Flux density measurement mode | 0.355 cps/($\mu\text{Sv} \cdot \text{h}^{-1}$) 0.355 cps/($\mu\text{Sv} \cdot \text{h}^{-1}$) 0.7 cps/($\mu\text{Sv} \cdot \text{h}^{-1}$) 0.5 cps/($\text{neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$) 0.5 cps/($\text{neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$) 10 cps/($\text{neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$) 1 cps/($\text{neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$) |
| Protection class | - all DUs | IP64 |
| Overall dimensions, weight | - BDKN-01 - BDKN-03 - BDKN-05 - BDKN-06 | $\varnothing 90 \times 260$ mm, 2 kg $316 \times 220 \times 265$ mm, 8 kg $105 \times 115 \times 380$ mm, 3.5 kg $550 \times 254 \times 254$ mm, 10 kg (w/o tripod) |

BDKN-06



AT1117M. Alpha radiation detection units



| | | |
|---|--|---|
| Detector | - BDPA-01 - BDPA-02 - BDPA-03 - BDPS-02 | ZnS(Ag) scintillator, 30 cm ² ZnS(Ag) scintillator, 100 cm ² ZnS(Ag) scintillator, 300 cm ² Geiger-Mueller counter tube |
| Measurement range of alpha particles flux density | - BDPA-01 - BDPA-02 - BDPA-03 - BDPS-02 | $0.1 - 10^5 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ $0.05 - 5 \cdot 10^4 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ $0.05 - 2 \cdot 10^4 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ $2.4 - 10^6 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ |
| Measurement range of ²³⁸ Pu surface activity | - BDPA-01 - BDPA-02 - BDPA-03 | $3.4 \cdot 10^{-3} - 3.4 \cdot 10^3 \text{ Bq} \cdot \text{cm}^{-2}$ $1.7 \cdot 10^{-3} - 1.7 \cdot 10^3 \text{ Bq} \cdot \text{cm}^{-2}$ $1.7 \cdot 10^{-3} - 0.68 \cdot 10^3 \text{ Bq} \cdot \text{cm}^{-2}$ |
| Limits of tolerable intrinsic relative error | - all DUs | ±20% |
| Energy range | - all DUs | 4 – 7 MeV |
| Typical sensitivity to ²³⁹ Pu radiation | - BDPA-01 - BDPA-02 - BDPA-03 - BDPS-02 | $0.15 \text{ cps}/(\text{particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2})$ $0.7 \text{ cps}/(\text{particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2})$ $2.5 \text{ cps}/(\text{particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2})$ $0.045 \text{ cps}/(\text{particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2})$ |
| Protection class | - all DUs | IP64 |
| Overall dimensions, weight | - BDPA-01 - BDPA-02 - BDPA-03 - BDPS-02 | Ø85x200 mm, 0.5 kg Ø137x230 mm, 0.7 kg Ø222x277 mm, 1.4 kg 138x86x60 mm, 0.33 kg |

AT1117M. Beta radiation detection units



| | | |
|--|--|---|
| Detector | - BDPB-01 - BDPB-02 - BDPB-03 - BDPS-02 | Scintillation plastic, 30 cm ² Scintillation plastic, 100 cm ² Scintillation plastic, 300 cm ² Geiger-Mueller counter tube |
| Measurement range of beta particles flux density | - BDPB-01 - BDPB-02 - BDPB-03 - BDPS-02 | $1 - 5 \cdot 10^5 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ $0.5 - 1.5 \cdot 10^5 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ $0.5 - 0.5 \cdot 10^5 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ $6 - 10^6 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ |
| Measurement range of ⁹⁰ Sr + ⁹⁰ Y surface activity | - BDPB-01 - BDPB-02 - BDPB-03 | $4.4 \cdot 10^{-2} - 2.2 \cdot 10^4 \text{ Bq} \cdot \text{cm}^{-2}$ $2.2 \cdot 10^{-2} - 0.66 \cdot 10^4 \text{ Bq} \cdot \text{cm}^{-2}$ $2.2 \cdot 10^{-2} - 0.22 \cdot 10^4 \text{ Bq} \cdot \text{cm}^{-2}$ |
| Limits of tolerable intrinsic relative error | - all DUs | ±20% |
| Energy range | - all DUs | 155 keV – 3.5 MeV |
| Typical sensitivity to ⁹⁰ Sr + ⁹⁰ Y radiation | - BDPB-01 - BDPB-02 - BDPB-03 - BDPS-02 | $0.3 \text{ cps}/(\text{particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2})$ $0.9 \text{ cps}/(\text{particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2})$ $2.4 \text{ cps}/(\text{particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2})$ $0.12 \text{ cps}/(\text{particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2})$ |
| Protection class | - all DUs | IP64 |
| Overall dimensions, weight | - BDPB-01 - BDPB-02 - BDPB-03 - BDPS-02 | Ø85x205 mm, 0.55 kg Ø137x235 mm, 0.87 kg Ø222x281 mm, 1.8 kg 138x86x60 mm, 0.33 kg |

AT1117M. Typical solutions

Remote measurements

- Detection unit (any except BDKN-03, BDKN-05, BDKN-06)
- PU / PU2 / PU4
- Telescopic bar (1.7 m / 3.2 m)



Control of hands and coats contaminated by alfa/beta particles



- PU2
- Detection unit (BDPA-02 / BDPA-03 / BDPB-02 / BDPB-03)



Handle for comfortable use

- Detection unit (any except BDKN-03, BDKN-05, BDKN-06)
- PU2
- Handle

Measurements with GPS-referencing

- Detection unit (any)
- PU4
- BT-DU4 Adapter



Mounting on a tripod

- Detection unit (any except BDKN-03, BDKN-05, BDKN-06)
- PU2 / PU4
- Tripod



Neutron dosimeter

- BDKN-03
- PU2 / PU4



Connection of alarm unit

- Detection unit (any)
- PU / PU2 / PU4
- Alarm unit

Sealed protective cases



Measurements in water, wells, etc.



- Detection unit (BDKG-01, BDKG-03, BDKG-04, BDKG-05, BDKG-17, BDKG-24, BDKG-30)
- PU / PU2 / PU4

AT2533, AT2533/1 Dosimeters



Measurement of ambient dose equivalent rate and ambient dose equivalent of continuous X-ray and gamma radiation in an extremely wide range and under harsh operating conditions, including emergency response.

Measurement of dose and average dose rate of pulsed radiation directly at linear accelerators (LINACs) and other pulsed radiation facilities.

- High burn-up life, rugged construction and integrity of detection unit
- Measurement in liquids at depths up to 40 m
- User friendly and easy to operate, highly available and can be used in gloves
- Instrument-to-PC data exchange over USB or Bluetooth interface (AT2533/1)
- The PU is able to control the radiation situation at operator location
- Available accessories: cable reel, wall brackets, etc.



Design and specifications are subject to change without notice

| | |
|---|---|
| Detector | Silicon semiconductor detector; Geiger-Muller counter tube |
| Energy range | 50 keV – 10 MeV |
| Measurement range of ambient dose equivalent rate $\dot{H}^*(10)$ | 1 $\mu\text{Sv/h}$ – 1000 Sv/h |
| Measurement range of ambient dose equivalent $H^*(10)$ | 10 μSv – 5000 Sv |
| Limits of variation of the response due to dose $H^*(10)$ and dose rate $\dot{H}^*(10)$ | $\pm 15\%$ |
| Measurement range of average pulsed radiation dose rate | 30 $\mu\text{Sv/s}$ – 0.3 Sv/s (100 mSv/h – 1000 Sv/h) (pulse repetition rate is not less than 20 cps, duration not less than 1 μs) |
| Measurement range of pulsed radiation dose | 10 μSv – 5000 Sv |
| Limits of variation of the response due to dose and average dose rate of pulsed radiation | $\pm 20\%$ |
| Limits of variation of relative response due to gamma radiation energy (50 keV to 3 MeV) and angle of incidence (0° to $\pm 45^\circ$) | -29% to +67% |
| Typical sensitivity to ^{137}Cs gamma radiation | 0.15 cps/ $(\mu\text{Sv}\cdot\text{h}^{-1})$ (for $\dot{H}^*(10) \leq 0.1$ Sv/h) 58 mV/ $(\text{Sv}\cdot\text{h}^{-1})$ (for $\dot{H}^*(10) > 0.1$ Sv/h) |
| Response time for 10-fold dose rate change | ≤ 10 s (for $\dot{H}^*(10) > 10$ $\mu\text{Sv/h}$) |
| Burn-up life | ≥ 25000 Sv (BDKG-33 and cable) |
| Protection class (BDKG-33) | IP68 (withstands static hydraulic pressure up to 400 kPa at 40 m immersion depth) |
| PC interface | USB 2.0 (AT2533) USB 2.0 / Bluetooth (AT2533/1) |
| Overall dimensions, weight | $\varnothing 30 \times 130$ mm, 0.25 kg (BDKG-33) 85x155x35 mm, 0.3 kg (PU-33) |

AT5350/1 Dosimeter

Highly functional precision dosimeter. Measurement of direct current rate, electric charge, charge by the method of numerical integration of current, air kerma and air kerma rate, kerma by the method of numerical integration of kerma rate and other radiological values.

Application:

- Metrology of ionizing radiation
- Measurement of low level current and charge
- Physical research of photon radiation fields
- Clinical dosimetry
- Radiation therapy
- Radiation protection



Delivery set:

- Electrometer measurement unit (Electrometer)
- Optional ionization chambers by PTW-Freiburg (Germany):
 - TM23342
Parallel-plane X-ray chamber (0.02 cm³)
 - TM31010
Cylindrical ionization chamber (0.125 cm³)
 - TM30010
Thimble ionization chamber (0.6 cm³)
 - TM23361
Cylindrical ionization chamber (30 cm³)
 - TM32002
Spherical ionization chamber (1000 cm³)

| | |
|---|--|
| Measurement range: - Direct current rate - Electric charge - Charge by the method of numerical integration of current | $1 \cdot 10^{-15} - 1 \cdot 10^{-6} \text{ A}$ $1 \cdot 10^{-15} - 1 \cdot 10^{-8} \text{ C}$ $1 \cdot 10^{-14} - 1 \cdot 10^{-1} \text{ C}$ |
| Measurement accuracy | $\leq (0.1 - 0.5)\%$ |
| Measurement range: - Air kerma rate - Air kerma - Air kerma by the method of numerical integration of kerma rate | $0.4 \mu\text{Gy/min} - 10 \text{ kGy/min}$ $0.05 \mu\text{Gy} - 15 \text{ Gy}$ $0.05 \mu\text{Gy} - 1.5 \text{ MGy}$ |
| Measurement accuracy | $\pm 3\% \text{ max}$ |
| X-ray and gamma radiation energy range | 8 keV – 1.33 MeV |
| Leakage current | $\leq 1 \cdot 10^{-15} \text{ A}$ |
| Integration time | <99999 s |
| Power supply | 230 VAC, 50 Hz |
| Power consumption | $\leq 12 \text{ V} \cdot \text{A}$ |
| Overall dimensions / weight | 294x112.5x250 mm / 3.8 kg |
| Integrated high voltage power source $\pm(1 - 500) \text{ V}$ for ionization chambers with 1 V setup steps | |
| Library of parameters for 20 ionization chambers | |
| Memory for up to 500 measurement results | |
| Automatic correction of measurement results taking into account air density for unpressurised chambers based on the entered temperature and pressure values | |
| Selectable unit of measurement (Gy, Sv, R, A, C) | |
| RS232C interface and dedicated digital inputs/outputs | |

Spectrometers (Radionuclide Identification Devices)

AT1321 Spectrometer (Spectrometric Personal Radiation Detector)



- Search and detect gamma radiation sources with identification of radionuclide composition
- Measure gamma radiation ambient dose equivalent rate
- Highly-sensitive to gamma radiation and compact
- Spectrum analysis and radionuclide identification without PC
- Integrated GPS module
- Sound, light and vibration notification
- "GARM" application software for further data processing and analysis in expert mode and radiological mapping



| | |
|---|---|
| Detectors | Scintillation, NaI(Tl) Ø25x40 mm Geiger-Muller counter tube |
| Energy range | 20 keV – 3 MeV |
| Detectable activity of ^{137}Cs source, located at the distance of 15 cm in a time not longer than 2 s | (50±10) kBq |
| Typical resolution at 662 keV (^{137}Cs) | 8% |
| Measurement range of ambient dose equivalent rate | 30 nSv/h – 100 mSv/h |
| Limits of tolerable intrinsic relative error | ±20% |
| Typical sensitivity to ^{137}Cs gamma radiation | 425 cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) |
| Energy dependence relative to 662 keV (^{137}Cs) | ±20% (50 keV to 3 MeV) |
| Response time for dose rate change from 0.1 to 1 $\mu\text{Sv/h}$ | <2 s |
| Protection class | IP54 |
| Overall dimensions, weight | 145x100x50 mm, 0.7 kg |



Design and specifications are subject to change without notice

Spectrometers (Radionuclide Identification Devices)

AT1120M, AT1120MA Spectrometers



- Quick search and detection of gamma radiation sources with identification of radionuclide composition
- Measurement of gamma radiation ambient dose equivalent rate
- High sensitivity and quick accommodation to changes in radiation level
- Short measurement cycle (1/3 s) provided by the search algorithm, enables highly confident estimation of rapidly changing radiation field dynamics and highly precise localization of radioactive sources
- Continuously recorded scanning data with GPS georeferencing
- Voice messaging option for identification results is available
- "GARM" application software for further data processing and analysis in expert mode and radiological mapping

| | | AT1120M | AT1120MA |
|---|-----------|---|---|
| Detection unit (DU) | | BDKG-11M | BDKG-05M |
| Processing unit (PU4) | | PU5 is a hand-held PC (HPC) with integrated detection module | |
| Detector | DU PU5 | Scintillation, NaI(Tl) Ø63x63 mm Geiger-Muller counter tube | Scintillation, NaI(Tl) Ø40x40 mm Geiger-Muller counter tube |
| Energy range | DU PU5 | 20 keV – 7 MeV 60 keV – 3 MeV | |
| Detectable activity of ^{137}Cs source, located at the distance of 20 cm in a time not longer than 2 s | DU | (30±6) kBq | (50±10) kBq |
| Typical resolution at 662 keV (^{137}Cs) | DU | 7.5% | |
| Measurement range of ambient dose equivalent rate | DU PU5 | 0.03 – 150 µSv/h 1 µSv/h – 100 mSv/h | 0.03 – 300 µSv/h 1 µSv/h – 100 mSv/h |
| Limits of intrinsic relative measurement error | DU PU5 | ±20% | |
| Typical sensitivity to ^{137}Cs gamma radiation | DU | 2700 cps/(µSv·h ⁻¹) | 870 cps/(µSv·h ⁻¹) |
| Energy dependence relative to 662 keV (^{137}Cs) | DU PU5 | ±15% (50 keV to 7 MeV) -25% to +35% (60 keV to 3 MeV) | |
| Response time for dose rate change from 0.1 to 1 µSv/h | DU | ≤2 s | |
| Protection class | DU PU5 | IP54 IP67 | |
| Overall dimensions, weight (assembled with handle) | | 355x190x170 mm, 2.65 kg | 330x180x160 mm, 1.85 kg |

Spectrometers (Radionuclide Identification Devices)

AT1120ME Spectrometer



- Quick search and detection of gamma radiation sources with identification of radionuclide composition
- Measurement of gamma radiation ambient dose equivalent rate
- $\text{SrI}_2(\text{Eu})$ scintillator with high energy resolution: 3.2% for 662 keV (^{137}Cs)
- Reliable identification of complex radionuclide mixtures
- High sensitivity and quick accommodation to changes in radiation level
- Short measurement cycle (1/3 s) provided by the search algorithm, enables highly confident estimation of rapidly changing radiation field dynamics and highly precise localization of radioactive sources
- IP67 dust proof and water resistant
- Continuously recorded scanning data with GPS georeferencing
- Voice messaging option for identification results is available
- "GARM" application software for further data processing and analysis in expert mode and radiological mapping



| Detection Unit (DU) | | BDKG-05S |
|---|-----------|--|
| Processing Unit (PU5) | | PU5 is a hand-held PC (HPC) with integrated detection module |
| Detector | DU PU5 | Scintillation $\text{SrI}_2(\text{Eu})$ Ø38x38 mm Geiger-Muller counter tube |
| Energy range | DU PU5 | 20 keV – 3 MeV 60 keV – 3 MeV |
| Detectable activity of ^{137}Cs source, located at the distance of 20 cm in a time not longer than 2 s | DU | (40±4) kBq |
| Typical resolution at 662 keV (^{137}Cs) | DU | 3.2% |
| Measurement range of ambient dose equivalent rate | DU PU5 | 0.04 – 150 µSv/h 1 µSv/h – 100 mSv/h |
| Limits of tolerable intrinsic relative error | DU PU5 | ±20% |
| Typical sensitivity to ^{137}Cs gamma radiation | DU | 850 cps/(µSv·h ⁻¹) |
| Energy dependence relative to 662 keV (^{137}Cs) | DU PU5 | ±20% (40 keV to 3 MeV) -25% to +35% (60 keV to 3 MeV) |
| Response time for dose rate change from 0.1 to 1 µSv/h | DU | ≤2 s |
| Protection class | | IP67 |
| Overall dimensions, weight (assembled with handle) | | 320x180x160 mm, 1.85 kg |

Design and specifications are subject to change without notice

Spectrometers (Radionuclide Identification Devices)



- Single-block design
- Multiple functions
- Integrated GPS module
- Sound, vibration and light alarm
- Connection of external detection units
- 25 hours (AT6102A, B) and 18 hours (AT6102) of battery operation time

AT6102, AT6102A, AT6102B Spectrometers

- Search and detection of gamma radiation sources with automatic identification of radionuclide composition
- Measurement of gamma radiation ambient dose equivalent rate
- Detection of neutron radiation and measurement of neutron count rate (AT6102)
- Measurement of neutron radiation dose rate (BDKN-03)
- Measurement of alpha and beta particles flux density from contaminated surfaces (BDPA-01/BDPB-01)

| | | |
|---|---------|--|
| Gamma radiation detectors | AT6102 | Nal(Tl) scintillator, Ø40x40 mm; Geiger-Mueller counter tube |
| | AT6102A | |
| | AT6102B | Nal(Tl) scintillator, Ø40x80 mm; Geiger-Mueller counter tube |
| Neutron radiation detector | AT6102 | Two ³ He-proportional neutron counters |
| Energy range - Gamma radiation - Neutron radiation | | 20 keV – 3 MeV 0.025 eV – 14 MeV (AT6102) |
| Detectable activity of ¹³⁷ Cs source, located at the distance of 20 cm in a time not longer than 2 s | | (50±10) kBq |
| Detectable activity of ²⁵² Cf source, located at the distance of 20 cm in a time not longer than 5 s | | 1.8·10 ⁴ neutron/s (Probability of detection is 0.9) |
| Typical resolution at 662 keV (¹³⁷ Cs) | | 7.5% (AT6102, A) 8% (AT6102B) |
| Measurement range of ambient dose equivalent rate | | 30 nSv/h – 100 mSv/h |
| Limits of tolerable intrinsic relative error | | ±20% |
| Typical sensitivity to ¹³⁷ Cs gamma radiation | | 850 cps/(μSv·h ⁻¹) (AT6102, A) 1700 cps/(μSv·h ⁻¹) (AT6102B) |
| Protection class | | IP65 |
| Overall dimensions, weight | | 230x115x212 mm, 2.5 kg (AT6102) 230x115x177 mm, 1.9 kg (AT6102A) 230x115x177 mm, 2.15 kg (AT6102B) |

| Detection unit | BDPA-01 (α) | BDPB-01 (β) | BDKN-03 (n) |
|---------------------|---|--|---|
| Detector | ZnS(Ag) scintillator, Ø60 mm | Scintillation plastic, Ø60 mm | ³ He counter in polyethylene moderator |
| Measurement range | 0.5 – 10 ⁵ particle·min ⁻¹ ·cm ⁻² (Flux density) | 3 – 5·10 ⁵ particle·min ⁻¹ ·cm ⁻² (Flux density) | 0.1 μSv/h – 10 mSv/h (Dose rate) |
| | Limits of intrinsic relative measurement error: ±20% | | |
| Energy range | 4 – 7 MeV | 155 keV – 3.5 MeV | 0.025 eV – 14 MeV |
| Typical sensitivity | 0.15 cps/(particle·min ⁻¹ ·cm ⁻²) [²³⁹ Pu] | 0.3 cps/(particle·min ⁻¹ ·cm ⁻²) [⁹⁰ Sr+ ⁹⁰ Y] | 0.355 cps/(μSv·h ⁻¹) [Pu-Be] |
| Dimensions, weight | Ø85x200 mm, 0.5 kg | Ø85x205 mm, 0.55 kg | 316x220x265 mm, 8 kg |
| Protection class | IP64 | IP64 | IP64 |
| Image | | | |

Design and specifications are subject to change without notice



Rugged HPC or tablet PC
for control and indication



AT6101DR Spectrometer

- Measurement of ^{134}Cs and ^{137}Cs surface contamination and specific activity in soils
- Automatic determination of soil layer thickness contaminated by ^{137}Cs and ^{134}Cs radionuclides
- Measurement of ^{137}Cs , ^{134}Cs and ^{131}I specific activity in water, foodstuffs, agricultural and forestry products and liquid radioactive wastes
- Determination of ^{40}K , ^{226}Ra and ^{232}Th natural radionuclides content
- Radionuclide identification: ^{134}Cs , ^{137}Cs , ^{131}I , ^{40}K , ^{226}Ra , ^{232}Th
- Measurement of gamma radiation ambient dose equivalent rate
- No-sampling measurement with GPS-referencing
- Smart detection unit in sealed container
- "GARM" application software for further data processing and analysis in expert mode and radiological mapping

| | |
|--|--|
| Scintillation detector | Nal(Tl) Ø63x63 mm |
| Energy range | 50 keV – 3 MeV |
| Measurement ranges (2π geometry) | |
| - Surface activity of ^{134}Cs and ^{137}Cs | 4 – 3700 kBq/m ² (0.1 – 100 Ci/km ²) |
| - Specific activity of ^{134}Cs and ^{137}Cs (<i>in situ</i>) | 50 – 10 ⁶ Bq/kg |
| - Specific effective activity of ^{40}K , ^{226}Ra , ^{232}Th | 100 – 10 ⁴ Bq/kg |
| Measurement ranges (4π geometry) | |
| - Specific activity of ^{134}Cs and ^{137}Cs | 50 – 10 ⁶ Bq/kg |
| - Specific activity of ^{131}I | 30 – 10 ⁶ Bq/kg |
| - Specific effective activity of ^{40}K , ^{226}Ra , ^{232}Th | 50 – 10 ⁴ Bq/kg |
| Typical resolution at 662 keV (^{137}Cs) | 8% |
| Measurement range of ambient dose equivalent rate | 0.03 – 130 µSv/h |
| Limits of tolerable intrinsic relative error of activity and dose rate measurement | ±20% |
| Typical sensitivity to ^{137}Cs gamma radiation | 2200 cps/(µSv·h ⁻¹) |
| Protection class | IP67 |
| Overall dimensions, weight | Ø130x500 mm, 4.5 kg |



Design and specifications are subject to change without notice

AT6104DM, AT6104DM1 Spectrometers




Rugged HPC or tablet PC
for control and indication

Radioactive contamination control of water and bottom sediments at depths up to 500 meters with GPS-referencing

- Determination of spatial position of detection device during measurement
- Cable reel with a current feedthrough
- Display of measurement results on index maps of controlled radionuclides concentration or gamma radiation dose rate distribution
- Expert mode for instrument spectrum analysis with automatic identification of sample radionuclide content
- Expert "GARM" software for further data processing and analysis, and radiological mapping



| | AT6104DM | AT6104DM1 |
|--|---|---|
| Scintillation detector | Nal(Tl) Ø63x63 mm | Nal(Tl) Ø63x160 mm |
| Energy range | 70 keV – 3 MeV | |
| Identified radionuclides | ¹³⁷ Cs, ¹³⁴ Cs, ¹³¹ I, ⁴⁰ K, ²²⁶ Ra, ²³² Th | |
| | Extended library (add ⁶⁰ Co, ²⁴ Na, ⁵⁴ Mn, etc.) available on request | |
| Measurement range of specific activity in water (4π geometry) | 3 – 1·10 ⁶ Bq/kg [¹³⁴ Cs, ¹³⁷ Cs, ¹³¹ I] 250 – 2·10 ⁴ Bq/kg [⁴⁰ K] | 1 – 1·10 ⁶ Bq/kg [¹³⁴ Cs, ¹³⁷ Cs, ¹³¹ I] 100 – 2·10 ⁴ Bq/kg [⁴⁰ K] |
| | Extended library (add ⁶⁰ Co, ⁵⁴ Mn, etc.) available on request | |
| Measurement range of specific activity in bottom sediments (2π geometry) | 50 – 1·10 ⁶ Bq/kg [¹³⁴ Cs, ¹³⁷ Cs] 250 – 2·10 ⁴ Bq/kg [⁴⁰ K] | – |
| Typical resolution at 662 keV (¹³⁷ Cs) | 7.5% | 8.5% |
| Measurement range of ambient dose equivalent rate | 0.03 – 130 μSv/h | 0.03 – 50 μSv/h |
| Limits of tolerable intrinsic relative error | ±20% (for specific activity and dose rate measurement) | |
| Typical sensitivity to ¹³⁷ Cs gamma radiation | 2350 cps/(μSv·h ⁻¹) | 5100 cps/(μSv·h ⁻¹) |
| Protection class of the detection device | IP68 (Withstands static hydraulic pressure up to 5 MPa for not less than 24 h) | |
| Overall dimensions and weight of detection device | Ø130x510 mm, 4.5 kg | Ø130x633 mm, 6.5 kg |

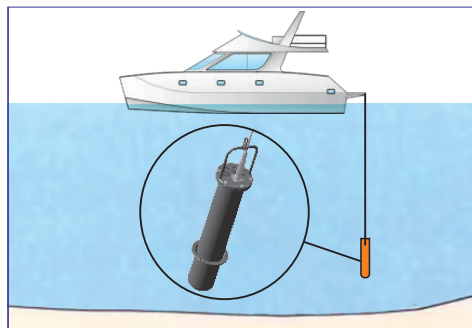

AT6101C, AT6101CM Spectrometers (Backpack-based Radiation Detectors)



Rugged Android smartphone (4.7" or 6") for control and indication

Inconspicuous search and detection of radiation sources with radionuclide identification.

Effective technical solution to prevent illicit traffic of radioactive materials.



- Shares leading market position
- 20 hours of operation time
- Automatic simultaneous gamma and neutron radiation scanning with radionuclide identification
- Continuous recording of scanning data with GPS-referencing for further analysis
- Dose rate measurement range can be expanded to 10 Sv/h
- Expert "GARM" software for further data processing and analysis
- Optional rugged case for spectrometer

| | AT6101C | AT6101CM |
|--|---|--|
| Gamma radiation detection units, scintillation detector | BDKG-11M (1 or 2 units), NaI(Tl) Ø63x63 mm | BDKG-19M (1 or 2 units), NaI(Tl) Ø63x160 mm |
| Energy range | 20 keV – 3 MeV | |
| Measurement range of ambient dose equivalent rate | 0.03 – 150 µSv/h | 0.03 – 50 µSv/h |
| | Limits of tolerable intrinsic relative error: ±20% | |
| Typical sensitivity to ¹³⁷ Cs gamma radiation | 2200 cps/(µSv·h ⁻¹) [4400 cps/(µSv·h ⁻¹)]* | 6000 cps/(µSv·h ⁻¹) [12000 cps/(µSv·h ⁻¹)]* |
| Detectable activity of ¹³⁷ Cs source, moving at the speed of 0.6 m/s and located at the distance of 1 m in a time not longer than 2 s | 400 kBq [280 kBq]* | 250 kBq [170 kBq]* |
| | 95% probability of source detection with false alarm rate not above 1 in 10 min | |
| Alarm activation time | <2 s | |
| Typical resolution at 662 keV (¹³⁷ Cs) | 7.5% | 8% |
| Identified radionuclides | Industrial, natural, medical (The library content can be modified on request) | |
| Option to extend the dose rate measurement range | BDKG-04 detection unit, up to 10 Sv/h | |
| Neutron radiation detection unit, detector | BDKN-05M** , Two He-3 proportional counters Ø30x360 mm in polyethylene moderator | |
| Energy range | 0.025 eV – 14 MeV | |
| Typical sensitivity to ²⁵² Cf neutron radiation | 20 cps/(neutron·s ⁻¹ ·cm ⁻²) | |
| Detectable activity of Pu-Be source, located at the distance of 1.25 m in a time not longer than 3 s | (5.00±1.25)·10 ⁴ neutron/s | |
| | 95% probability of source detection with false alarm rate not above 1 in 1 h | |
| Protection class | IP55 (in a backpack) / IP65 (in a case) | |
| Overall dimensions, weight *** | in a backpack in a case | 550x340x220 mm, 9 kg 625x500x300 mm, 18 kg |
| | 520x380x220 mm, 7 kg 625x500x300 mm, 16.5 kg | |

* Configuration with two BDKG-11M (BDKG-19) detection units

** Not available for configuration with two BDKG-11M (BDKG-19) detection units

*** Configuration with BDKG-11M (BDKG-19M) and BDKN-05M detection units

Design and specifications are subject to change without notice

AT6101CE Spectrometer (Backpack-based Radiation Detector)



Rugged Android smartphone (4.7" or 6") for control and indication

Inconspicuous search and detection of radiation sources with radionuclide identification.

Effective technical solution to prevent illicit traffic of radioactive materials.



- $\text{SrI}_2(\text{Eu})$ scintillator with high energy resolution: 3.2% for 662 keV (^{137}Cs)
- Reliable identification of complex radionuclide mixtures
- 20 hours of operation time
- Automatic simultaneous gamma and neutron radiation scanning with radionuclide identification
- Continuous recording of scanning data with GPS-referencing for further analysis
- Expert "GARM" software for further data processing and analysis
- Optional rugged case for spectrometer

| AT6101CE | | |
|--|----------------------------|--|
| Gamma radiation detection units, scintillation detector | | BDKG-05S , $\text{SrI}_2(\text{Eu})$ $\varnothing 38 \times 38$ mm BDKG-35 , plastic $\varnothing 70 \times 150$ mm |
| Energy range | | 20 keV – 3 MeV |
| Measurement range of ambient dose equivalent rate | | 0.03 – 150 $\mu\text{Sv/h}$ |
| | | Limits of tolerable intrinsic relative error: $\pm 20\%$ |
| Typical sensitivity to ^{137}Cs gamma radiation | | 4500 cps/($\mu\text{Sv} \cdot \text{h}^{-1}$) |
| Detectable activity of ^{137}Cs source, moving at the speed of 0.6 m/s and located at the distance of 1 m in a time not longer than 2 s | | 350 kBq |
| | | 95 % probability of source detection with false alarm rate not above 1 in 10 min |
| Alarm activation time | | <2 s |
| Typical resolution at 662 keV (^{137}Cs) | | 3.2% (BDKG-05S) |
| Identified radionuclides | | Industrial, natural, medical (The library content can be modified on request) |
| | | |
| Neutron radiation detection unit, detector | | BDKN-05M , Two He-3 proportional counters $\varnothing 30 \times 360$ mm in polyethylene moderator |
| Energy range | | 0.025 eV – 14 MeV |
| Typical sensitivity to ^{252}Cf neutron radiation | | 20 cps/(neutron $\cdot \text{s}^{-1} \cdot \text{cm}^2$) |
| Detectable activity of Pu-Be source, located at the distance of 1.25 m in a time not longer than 3 s | | $(5.00 \pm 1.25) \cdot 10^4$ neutron/s |
| | | 95% probability of source detection with false alarm rate not above 1 in 1 h |
| Protection class | in a backpack in a case | IP55 IP65 |
| Overall dimensions, weight | in a backpack in a case | 520X380x220 mm, 7.5 kg 594X473x215 mm, 16 kg |

AT6103 Mobile Radiation Scanning System



Radiation survey of the area in real time and search for gamma and neutron radiation sources with GPS-referencing

The system can be mounted on a motor vehicle, marine vessel or aircraft without any special tools



- User-selectable set of smart detection units
- High system scalability in terms of sensitivity to gamma and neutron radiation
- Automatic simultaneous gamma and neutron radiation scanning
- Real-time display of measurement results with GPS-referencing
- Search and detection of radioactive sources and real-time identification of its isotopic composition
- Storage and operation in rugged cases
- Assessment of surface contamination with ^{137}Cs radionuclide ($\text{kBq/m}^2, \text{Ci/km}^2$)
- "GARM" application software for further data processing and analysis in expert mode and radiological mapping
- "ARMS" application software for automatic transfer of data to a remote server (option)



Rugged 10" tablet PC for control and indication



Highly-sensitive gamma radiation and neutron radiation monitor: BDKG-28 (1 unit), BDKN-05 (2 units)



Highly-sensitive gamma radiation and neutron radiation counting monitor: BDRM-05 (1 unit), BDKN-05 (2 units)



Gamma radiation and neutron radiation monitor: BDKG-11M (1 unit), BDKG-04 (1 unit), BDNG-05 (1 unit)



Accessories

Available monitors

[Each monitor may contain 1 – 3 detection units (DU)]

[The configuration of the system is user-defined]

- 1) Gamma radiation and neutron radiation monitor** [1 – 3 units of BDKG -11M and/or BDKG-19M, 1 – 2 units of BDKN-05, 1 unit of BDKG-04]
- 2) Highly-sensitive gamma radiation and neutron radiation monitor** [1 – 3 units of BDKG-28 and/or BDKG-34, 1 – 3 units of BDKN-05, 1 unit of BDKG-04]
- 3) Highly-sensitive gamma radiation and neutron radiation counting monitor** [1 – 2 units of BDRM-05, 1 – 2 units of BDKN-05, 1 unit of BDKG-04]

| | |
|--|---|
| Total number of monitors in the system | 18 |
| Identified radionuclides | Medical, industrial and natural (The library content can be modified on request) |
| Continuous run time | ~ 10 h (With lowest brightness of Tablet PC screen) |
| Protection class | IP55 |

Radiation Scanning Equipment

AT6103 Mobile Radiation Scanning System

| Gamma radiation detection unit | | BDKG-11M | BDKG-19M | BDKG-04 | BDKG-28 | BDKG-34 | BDRM-05 |
|--|-------------------|--|--------------------------|---|---------------------------|--------------------------|--|
| Scintillation detector | | Nal(Tl) Ø63x63 mm | Nal(Tl) Ø63x160 mm | Plastic Ø30x15 mm | Nal(Tl) 400x100x100 mm | Nal(Tl) 400x100x50 mm | Plastic 1000x100x50 mm |
| Energy range | | 20 keV – 3 MeV | 20 keV – 3 MeV | 15 keV – 3 MeV | 50 keV – 3 MeV | 30 keV – 3 MeV | 50 keV – 3 MeV |
| Measurement range of ambient dose equivalent rate | | 30 nSv/h – 150 µSv/h | 30 nSv/h – 50 µSv/h | 50 nSv/h – 10 Sv/h | 30 nSv/h – 7 µSv/h | 30 nSv/h – 10 µSv/h | Count rate indication range 0 – 5·10 ⁵ s ⁻¹ |
| | | Limits of tolerable intrinsic relative error: ±20% | | | | | |
| Typical sensitivity, cps/(µSv·h ⁻¹) | ²⁴¹ Am | 13500 | 37000 | 370 | 130000 | 118000 | 60000 |
| | ¹³⁷ Cs | 2200 | 6000 | 70 | 33000 | 26500 | 32000 |
| | ⁶⁰ Co | 1200 | 2500 | 40 | 19000 | 15500 | 17000 |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | | ±15% (50 keV - 3 MeV) | ±15% (50 keV - 3 MeV) | ±35% (15 - 60 keV) ±25% (60 keV - 3 MeV) | ±20% (50 keV - 3 MeV) | ±20% (50 keV - 3 MeV) | – |
| Response time for dose rate change from 0.1 to 1 µSv/h | | <2 s | <2 s | <3 s | <2 s | <2 s | – |
| Typical resolution at 662 keV (¹³⁷ Cs) | | 7.5 % | 8 % | – | 8.5 % | 8.5 % | – |

The system in “Search” mode detects the ¹³⁷Cs source of gamma radiation in less than 2 s in the following conditions:

| Gamma radiation detection unit | BDKG-11M | BDKG-19M | BDKG-28 | BDKG-34 | BDRM-05 |
|---|----------------|--------------|-------------|-------------|-------------|
| Source activity | (450±10) kBq | (300±10) kBq | (105±5) kBq | (105±5) kBq | (100±5) kBq |
| Distance from source to surface of detection unit | (100.0±0.5) cm | | | | |
| Detection probability | 95% | | | | |
| False alarm rate | ≤1 / 10 min | | | | |

| Neutron radiation detection unit | BDKN-05 |
|--|--|
| Detector | Two He-3 proportional counters Ø30x360 mm in polyethylene moderator |
| Indication range of neutron radiation impulse count rate | 0 – 2.5 · 10 ⁴ s ⁻¹ |
| Energy range | 0.025 eV – 14 MeV |
| Typical sensitivity to source radiation at the distance of 1 m, cps/(neutron·s ⁻¹ ·cm ⁻²) | 8 (Pu-Be) 20 (²⁵² Cf) |

The system in "Search" mode detects the Pu-Be source of neutron radiation in less than 3 s in the following conditions:

| Neutron radiation detection unit | BDKN-05 |
|---|---|
| Average neutron flux from source to solid angle 4π sr | (5.00±1.25) · 10 ⁴ neutron/s |
| Distance from source to surface of detection unit | (125±1) cm |
| Detection probability | 95% |
| False alarm rate | ≤1 / 1 h |

Design and specifications are subject to change without notice



AT1320A,B
with processing
unit



AT1320C

AT1320, A, B, C Gamma Activity Monitors

Measurement of volume activity and specific activity of gamma emitting radionuclides in water, foodstuff, agricultural raw materials and fodder, industrial raw materials, forestry products, building materials, soil and other objects of environment

- Smart spectrometric detection unit
- AT1320B: Radiation control of mushrooms and berries in 10-litre shipping box takes only 60 s
- AT1320C: Preliminary analysis of sample radionuclide composition in the process of measurement. Calculation of sample radionuclide activity on the basis of identification results
- Ready-to-use measurement procedures



| | | |
|--|---|---|
| Scintillation detector | | Nal(Tl) Ø63x63 mm |
| Energy range | | 50 keV – 3 MeV |
| Measurement range of volume (specific) activity | ¹³¹ I ¹³⁴ Cs ¹³⁷ Cs ⁴⁰ K ²²⁶ Ra ²³² Th | 3 – 1·10 ⁶ Bq/l (Bq/kg) 3 – 1·10 ⁶ Bq/l (Bq/kg) 3.7 – 1·10 ⁶ Bq/l (Bq/kg) 50 – 2·10 ⁴ Bq/l (Bq/kg) 10 – 1·10 ⁴ Bq/l (Bq/kg) 10 – 1·10 ⁴ Bq/l (Bq/kg) |
| Limits of tolerable intrinsic relative error | | ±20% |
| Density range of controlled samples | | 0.1 – 3 g/cm ³ |
| Typical resolution at 662 keV (¹³⁷ Cs) | | 8.5% |
| Number of ADC channels | | 512 / 1024 (AT1320C) |
| Overall dimensions, weight | Detection unit Processing unit Protection unit | Ø97x350 mm, 2 kg 200x106x35 mm, 0.62 kg Ø600x700 mm, 125 kg |
| Measurement geometry | Marinelli beaker Flat vessel Plastic box, 380x280x100 mm | 1 and 0.5 litre 0.5 and 0.1 litre 10 litre |

| | Controlled radionuclides | Control and indication | Measurement vessels |
|---------|---|---|--|
| AT1320 | ¹³⁷ Cs, ⁴⁰ K, ²²⁶ Ra, ²³² Th | Processing unit or External PC (option) | 1, 0.5 and 0.1 litre |
| AT1320A | ¹³⁷ Cs, ⁴⁰ K | | 1, 0.5 and 0.1 litre |
| AT1320B | ¹³⁷ Cs, ⁴⁰ K | | 1, 0.5, 0.1 and 10 litre (w/o protection unit lid) |
| AT1320C | ¹³¹ I, ¹³⁴ Cs, ¹³⁷ Cs, ⁴⁰ K, ²²⁶ Ra, ²³² Th | External PC (option) | 1, 0.5 and 0.1 litre |



AT1135 Portable Radiometric Laboratory

- Specific activity measurement of gamma-emitting ¹³⁴Cs, ¹³⁷Cs, ⁴⁰K radionuclides in food products
- In situ measurement of gamma radiation ambient dose equivalent rate

| | |
|--|--|
| Scintillation detector | Nal(Tl) Ø25x40 mm |
| Energy range | 50 keV – 1.5 MeV |
| Measurement range of specific activity for samples with 1 g/cm ³ density (measurement geometry: 0.5-litre Marinelli beaker) | 25 – 1·10 ⁵ Bq/kg (¹³⁴ Cs) 25 – 1·10 ⁵ Bq/kg (¹³⁷ Cs) 360 – 2·10 ⁴ Bq/kg (⁴⁰ K) |
| Density range of measured samples | 0.5 – 1.5 g/cm ³ |
| Dose rate measurement range | 0.03 – 300 µSv/h |
| Overall dimensions, weight | 200x200x437 mm, 14 kg |
| Control and indication | External PC (option) |

AT1315 Gamma Beta Spectrometer



Gamma Beta Spectrometer



Gamma Spectrometer

Simultaneous and selective activity measurement of gamma emitting radionuclides in potable water, food, agricultural raw materials and fodder, building materials, industrial raw materials, forestry products, soil and other objects of environment

Support of quick radioactive purity test for standardized sample metal heats

- Computer processing of spectra by means of maximum likelihood method
- Automatic allowance for sample density
- Simultaneous metering and processing of spectra
- Ready-to-use measurement procedures



| | | |
|--|--|---|
| Scintillation detector | <i>Gamma channel</i> <i>Beta channel</i> | Nal(Tl), Ø63x63 mm Plastic, Ø128x9 mm |
| Control and indication | External PC (<i>option</i>) | |
| Energy range | <i>Gamma radiation</i> <i>Beta radiation</i> | 50 keV – 3 MeV 150 keV – 3.5 MeV |
| Measurement range of volume (specific) activity without sample concentration (Spectrometric and radiometric measurement modes) | ^{137}Cs ^{40}K ^{232}Th , ^{226}Ra ^{90}Sr (Radiometric mode only) ^{131}I (Spectrometric mode only) ^{134}Cs (Spectrometric mode only) | 1 – 10^6 Bq/l (Bq/kg) 20 – $2 \cdot 10^4$ Bq/l (Bq/kg) 3 – 10^4 Bq/l (Bq/kg) 10 – 10^6 Bq/l (Bq/kg) 10 – 10^5 Bq/l (Bq/kg) 6 – 10^5 Bq/l (Bq/kg) |
| Limits of tolerable intrinsic relative error | ±20% | |
| Density range of controlled samples | 0.2 – 1.6 g/cm ³ | |
| Lower limit of ^{90}Sr measurement range with sample concentration in conversion to "wet" sample | 0.1 Bq/l 0.8 Bq/l 1.0 Bq/kg | |
| - For potable water - For milk, baby food - For potatoes, corn, grain and agricultural raw materials | | |
| Typical resolution at 662 keV (^{137}Cs) | 8% | |
| Number of ADC channels | 1024 | |
| Power supply | PC USB port | |
| Overall dimensions, weight (<i>Protection unit with gamma and beta radiation detection units</i>) | Ø474x910 mm, 194 kg | |
| Volume of measurement vessels | <i>For "wet" samples</i> <i>For concentrated samples</i> | Marinelli beaker 1 l, Flat vessels 0.5 and 0.1 l Flat vessels 0.2 and 0.03 l |



AT1329, AT1329A, AT1329B Sample Counters

Smear radiometry and simultaneous or independent measurement of gross alpha and beta activity in aerosol filters, counting samples

| | | |
|--|------------------|---|
| Scintillation detector | AT1329 | Phoswich detector (α and β channel): 28 cm ² , plastic with a layer of ZnS(Ag) |
| | AT1329A | ZnS(Ag) 28 cm ² (α channel) |
| | AT1329B | Plastic 28 cm ² (β channel) |
| Control and indication | | External PC (<i>option</i>) |
| Sensitivity | α channel | $\geq 0.25 \text{ Bq}^{-1} \cdot \text{s}^{-1}$ (^{239}Pu) |
| | β channel | $\geq 0.30 \text{ Bq}^{-1} \cdot \text{s}^{-1}$ ($^{90}\text{Sr} + ^{90}\text{Y}$) |
| Energy range | α channel | 3 – 7 MeV |
| | β channel | 155 keV – 3.5 MeV |
| Count rate measurement range | α channel | 0 – 10^5 s^{-1} |
| | β channel | 0 – 10^5 s^{-1} |
| Gross activity measurement range | α channel | $0.01 - 10^4 \text{ Bq}$ |
| | β channel | $0.1 - 10^4 \text{ Bq}$ |
| Background count rate | α channel | $\leq 0.001 \text{ s}^{-1}$ |
| | β channel | $\leq 0.75 \text{ s}^{-1}$ |
| Limits of tolerable intrinsic relative error | | $\pm 20\%$ |
| Protection class | | IP43 |
| Overall dimensions | | 230x230x290 mm |
| Weight | AT1329 | $\leq 22 \text{ kg}$ |
| | AT1329A | $\leq 10 \text{ kg}$ |
| | AT1329B | $\leq 22 \text{ kg}$ |



- Custom calibration settings
- Selectable units of measurement
- LED stabilization of measuring paths
- Automatic subtraction of external background
- Passive background radiation protection – lead shield (30 mm)
- Memory for measurement results
- Ready-to-use measurement procedures

Available configurations:

- AT1329 (*alpha-beta*)
- AT1329A (*alpha*)
- AT1329B (*beta*)





AT1316 (AT1316A) and AT1322 (AT1322/1) can be used in combination

WBCs can be installed into a van as part of mobile radiation monitoring laboratory



AT1316 Whole Body Counter

Activity measurement of ^{137}Cs and ^{134}Cs gamma-emitting radionuclides in human body.

- Calculation of expected annual effective internal exposure dose for incorporated ^{137}Cs and ^{134}Cs radionuclides
- Flexible software function controls, database and report generation on the basis of measurement results
- Express test productivity is 15 persons/hour



| | |
|---|--|
| Scintillation detector | Nal(Tl), Ø150x100 mm |
| Energy range | 50 keV – 3 MeV |
| Measurement range of activity | 80 – 7.5·10 ⁵ Bq (^{137}Cs) 80 – 4·10 ⁵ Bq (^{134}Cs) |
| Minimum measurable activity of ^{137}Cs and ^{134}Cs in adult body in 3 min | 300 Bq |
| Limits of tolerable intrinsic relative error | ±15% |
| Weight | 250 kg |

AT1316A Whole Body Counter

Activity measurement of ^{60}Co and other gamma-emitting radionuclides in human lungs.

- Control of gross activity threshold exceeding for ^{51}Cr , ^{54}Mn , ^{58}Co , ^{59}Fe , ^{65}Zn , ^{95}Nb , $^{100\text{m}}\text{Ag}$, ^{103}Ru , ^{124}Sb , ^{141}Ce , ^{144}Ce radionuclides in lungs
- Flexible software function controls, database and report generation on the basis of measurement results
- Express test productivity is 15 persons/hour



| | |
|---|--|
| Scintillation detector | Nal(Tl), Ø150x100 mm |
| Energy range | 50 keV – 2 MeV |
| Measurement range of activity | 40 – 1·10 ⁵ Bq (^{60}Co) |
| Minimum measurable activity of ^{60}Co in adult lungs in 3 min | 60 Bq |
| Limits of tolerable intrinsic relative error | ±20% |
| Weight | 250 kg |

AT1322, AT1322/1 Whole Body Counters


Activity measurement of ^{131}I and ^{133}I gamma-emitting radionuclides in human thyroid gland.

- Flexible software function controls, database and report generation on the basis of measurement results
- Express test productivity is 15 persons/hour



| | | |
|--|--------------------|---|
| Scintillation detector | AT1322 AT1322/1 | Nal(Tl), Ø40x40 mm Nal(Tl), Ø63x63 mm |
| Energy range | | 50 keV – 1.5 MeV |
| Measurement range of activity | AT1322 AT1322/1 | 85 – 10 ⁵ Bq (^{131}I) / 110 – 10 ⁵ Bq (^{133}I) 30 – 10 ⁵ Bq (^{131}I) / 40 – 10 ⁵ Bq (^{133}I) |
| Minimum measurable activity of ^{131}I and ^{133}I in the thyroid gland in 3 min | AT1322 AT1322/1 | 200 Bq (^{131}I) / 240 Bq (^{133}I) 80 Bq (^{131}I) / 100 Bq (^{133}I) |
| Limits of tolerable intrinsic relative error | | ±20% |
| Weight | | 70 kg |

AT2327 Alarm Dosimeter

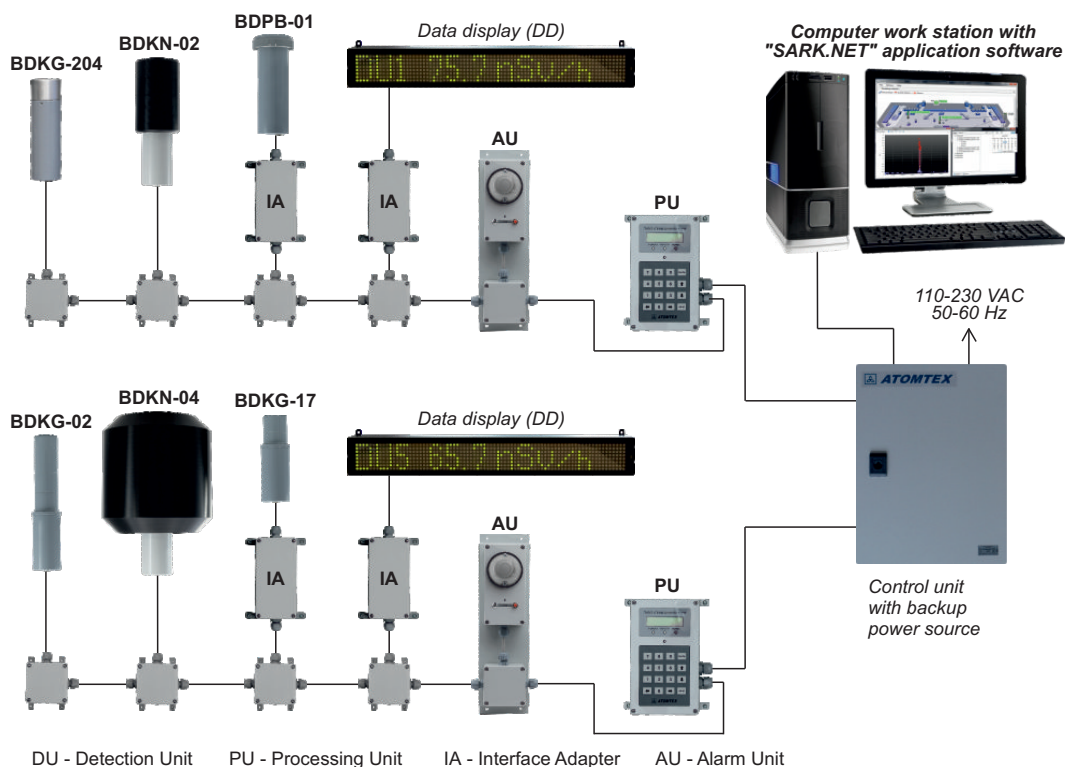

Sample functional chart of **AT2327 Alarm Dosimeter**

Radiation control of:

- radiation-sensitive and radiation-dangerous sites and facilities
- environment
- restricted area beamline at linear accelerators (LINACs) and other pulsed-radiation facilities

- Building a flexible and reliable multichannel stationary system
- Independent measurements of wide range gamma and neutron radiation dose rate and flux density of neutron and beta particles for each channel
- Sound and light alarm
- Self-check function
- Software for displaying current radiation environment in controlled area on PC screen
- Data logging
- Backup power source
- Integration into external security systems



| | |
|---|---|
| Number of detection units in one alarm dosimeter | 1 – 10 |
| Number of alarm dosimeters in the system for PC configuration | Up to 32 |
| Distance between detection unit and processing unit/PC when interface cable is used | 1000 m |
| Burn-up life | ≥ 100 Sv $\geq 10^8$ Sv (BDKG-27) $\geq 5 \cdot 10^4$ Sv (UDKG-37/2) |

Design and specifications are subject to change without notice

AT2327 Alarm Dosimeter


| | | |
|---|--|---|
| Detector | <ul style="list-style-type: none"> - BDKG-02 / -17 - BDKG-204 - BDKG-11 - BDKG-27 - UDKG-37/2 - BDPB-01 - BDKN-02 / -04 | Geiger-Mueller counter tube Scintillation plastic, Ø30x15 mm NaI(Tl) scintillator, Ø63x63 mm Ion chamber Silicon semiconductor detector + Geiger-Mueller counter tube Scintillation plastic, 30 cm ² He-3 counter in polyethylene moderator |
| Measurement range of gamma radiation ambient dose equivalent rate | <ul style="list-style-type: none"> - BDKG-02 - BDKG-204 - BDKG-11 - BDKG-17 - BDKG-27 - UDKG-37/2 | 0.1 µSv/h – 10 Sv/h 0.05 µSv/h – 10 Sv/h 0.03 – 100 µSv/h 1 mSv/h – 100 Sv/h 50 mSv/h – 4000 Sv/h 1 µSv/h – 5000 Sv/h |
| Measurement range of gamma radiation average pulsed radiation dose rate | - UDKG-37/2 | 30 µSv/s – 0.3 Sv/s (100 mSv/h – 1000 Sv/h) (pulse repetition rate is not less than 20 cps, duration not less than 1 µs) |
| Measurement range of ambient neutron radiation dose equivalent rate | <ul style="list-style-type: none"> - BDKN-02 - BDKN-04 | 0.1 µSv/h – 10 mSv/h [From Pu-Be source] 0.1 µSv/h – 10 mSv/h |
| Measurement range of beta particles flux density | - BDPB-01 | $1 - 5 \cdot 10^5 \text{ particle} \cdot \text{min}^{-1} \cdot \text{cm}^{-2}$ |
| Measurement range of neutron flux density | <ul style="list-style-type: none"> - BDKN-02 - BDKN-04 | $0.1 - 10^4 \text{ neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$ $0.1 - 10^4 \text{ neutron} \cdot \text{s}^{-1} \cdot \text{cm}^{-2}$ [From Pu-Be source] |
| Energy range of gamma radiation | <ul style="list-style-type: none"> - BDKG-02 - BDKG-11 - BDKG-17 - BDKG-27 - BDKG-204 - UDKG-37/2 | 60 keV – 3 MeV 50 keV – 3 MeV 60 keV – 3 MeV 60 keV – 1.5 MeV 20 keV – 10 MeV 50 keV – 10 MeV |
| Energy range of beta radiation | - BDPB-01 | 155 keV – 3.5 MeV |
| Energy range of neutron radiation | - BDKN-02 / -04 | 0.025 eV – 14 MeV |
| Typical sensitivity to ¹³⁷ Cs gamma radiation | <ul style="list-style-type: none"> - BDKG-02 - BDKG-204 - BDKG-11 - BDKG-17 - BDKG-27 - UDKG-37/2 | 4.0 cps/(µSv·h ⁻¹) 70.0 cps/(µSv·h ⁻¹) 1970 cps/(µSv·h ⁻¹) 0.005 cps/(µSv·h ⁻¹) 2.1 µC/Sv 0.15 cps/(µSv·h ⁻¹), for dose rate ≤0.2 Sv/h 58 mV/(Sv·h ⁻¹), for dose rate >0.2 Sv/h |
| Typical sensitivity to ⁹⁰ Sr+ ⁹⁰ Y beta radiation | - BDPB-01 | 0.3 cps/(particle·min ⁻¹ ·cm ⁻²) |
| Typical sensitivity to Pu-Be neutron radiation | <ul style="list-style-type: none"> - BDKN-02 / -04 - BDKN-02 / -04 | 0.5 cps/(neutron·s ⁻¹ ·cm ⁻²) 0.355 cps/(µSv·h ⁻¹) |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | <ul style="list-style-type: none"> - BDKG-02 - BDKG-11 - BDKG-17 - BDKG-27 - UDKG-37/2 - BDKG-204 | -20% to +35% ±20% -25% to +35% ±30% ±30% -45% to +35% (20 - 60 keV), ±25% (60 keV - 3 MeV) ±50% (3 - 10 MeV) |

Design and specifications are subject to change without notice

AT2327 Alarm Dosimeter

| | | |
|----------------------------|--|--|
| Protection class | <ul style="list-style-type: none"> - BDKG-02 - BDKG-11 - BDKG-17 - BDKG-27 - BDKG-204 - UDKG-37/2 - BDPB-01 - BDKN-02 - BDKN-04 - PU - AU - DD | <ul style="list-style-type: none"> IP57 IP65 (In sealed container) IP64 IP65 (Processing unit) IP65 (Ion chamber) IP67 IP68 (Detection unit) IP65 (Interface unit) IP64 IP54 IP54 IP55 IP65 IP21 |
| Overall dimensions, weight | <ul style="list-style-type: none"> - BDKG-02 - BDKG-11 - BDKG-17 - BDKG-27 - BDKG-204 - UDKG-37/2 - BDPB-01 - BDKN-02 - BDKN-04 - PU - AU - DD | <ul style="list-style-type: none"> Ø55x260 mm, 0.5 kg Ø141x473 mm, 6.5 kg (In sealed container) Ø54x167mm, 0.27kg 206x82x56 mm, 0.45 kg (Processing unit) 190x58x65 mm, 0.7 kg (Ion chamber) Ø60x210 mm, 0.55 kg Ø30x130 mm, 0.25 kg (Detection unit) 170x80x55 mm, 0.3 kg (Interface unit) Ø85x205 mm, 0.55 kg Ø91x260 mm, 2.4 kg 235x264x315 mm, 8 kg 200x160x90 mm, 0.7 kg 183x103x98 mm, 0.4 kg 644x98x67 mm, 4 kg |

AT2327 Alarm Dosimeter with Data Display



Gamma radiation detection unit (DU)




Control of radiation-sensitive and radiation-dangerous sites and territories with visual display of readings on a large screen.

- Logging of dose rate levels and threshold exceeding events
- The distance between the screen and a detection unit with temperature probe can be up to 1 km
- Additional protection from direct weather effects

| | |
|--|--|
| Detector | Geiger-Mueller counter tube |
| Energy range | 60 keV – 3 MeV |
| Measurement range of ambient dose equivalent rate | 0.1 µSv/h – 10 Sv/h |
| Typical sensitivity to ¹³⁷ Cs gamma radiation | 4 cps/(µSv h ⁻¹) |
| Visual display of data on screen | Dose rate, temperature, current date and time |
| Screen readability | 30 m at any time of day |
| Protection class | IP57 (DU), IP53 (Display) IP31 (Control unit) |
| Dimensions, weight | <i>Display with DU</i> 1095x392x300 mm, 25 kg <i>Control unit</i> 500x650x150 mm, 30 kg |

AT2341 Radiation Monitoring Station

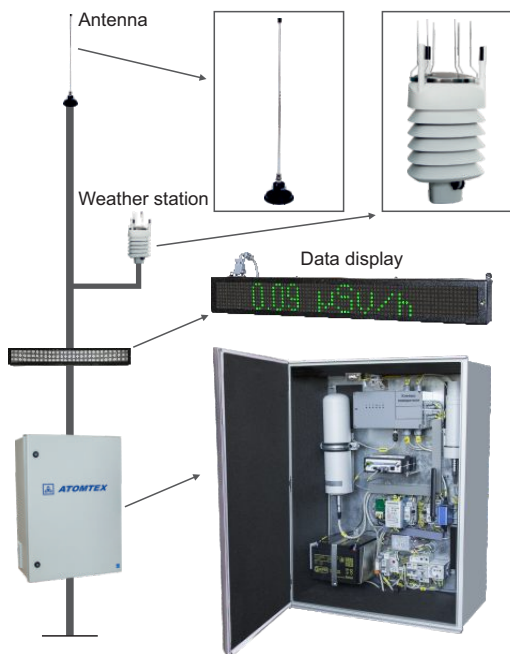

Continuous radiation and weather control in the zone of influence of nuclear power plants and other radiation-hazardous facilities.

Combine stations into a single network (up to 256 units) and use dedicated software to build an automated radiation situation monitoring system.

- High-sensitive spectrometric measurement channel
- Simultaneous monitoring of radiation and weather data
- Redundant power supply for at least 72 hours operation time
- Communication links: Cellular (3G, 4G, 5G); Ethernet; Wireless; Wi-Fi

| | |
|-----------------------------|---|
| Protection rating | IP65 (IP66 for weather station) |
| Operation temperature range | -40...+50°C |
| Relative air humidity | ≤98% (Air temperature ≤35°C without condensation) |
| Dimensions | 800x600x300 mm |
| Weight | ≤45 kg |


SPECTROMETRIC CHANNEL

| Detection unit | BDKG-211M |
|--|---|
| Detector | NaI(Tl) scintillator, Ø63x63 mm |
| Energy range | 20 keV – 3 MeV |
| Measurement range of ambient dose equivalent rate | 30 nSv/h – 150 μSv/h |
| Limits of tolerable intrinsic relative error | ±20% |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | ±20% (40 keV – 3 MeV) |
| Typical sensitivity to gamma radiation, cps/(μSv·h ⁻¹) | 13900 (²⁴¹ Am) / 2450 (¹³⁷ Cs) / 1300 (⁶⁰ Co) |
| Response time for dose rate change from 0.1 to 1 μSv/h | ≤2 s |
| Typical resolution at 662 keV (¹³⁷ Cs) | 7.5% |

DOSIMETRIC CHANNEL (available options)

| Detection unit | BDKG-22 | BDKG-224 |
|--|---|--|
| Detector | Geiger-Muller counter tube | Tissue-equivalent scintillation plastic, Ø50x40 mm |
| Energy range | 60 keV – 3 MeV | 30 keV – 10 MeV |
| Measurement range of ambient dose equivalent rate | 100 nSv/h – 10 Sv/h | 40 nSv/h – 1 Sv/h |
| | Limits of tolerable intrinsic relative error: ±20% | |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | -25% to +35% (60 keV – 3 MeV) | ±25% (30 keV – 3 MeV) ±40% (3 – 10 MeV) |
| Typical sensitivity to gamma radiation, cps/(μSv·h ⁻¹) | 4 (²⁴¹ Am) 4 (¹³⁷ Cs) 4 (⁶⁰ Co) | 3200 (²⁴¹ Am) 530 (¹³⁷ Cs) 270 (⁶⁰ Co) |
| Response time for dose rate change from 0.1 to 1 μSv/h | ≤7 s | ≤2 s |

AT2331 Emergency Alarm Dosimeter

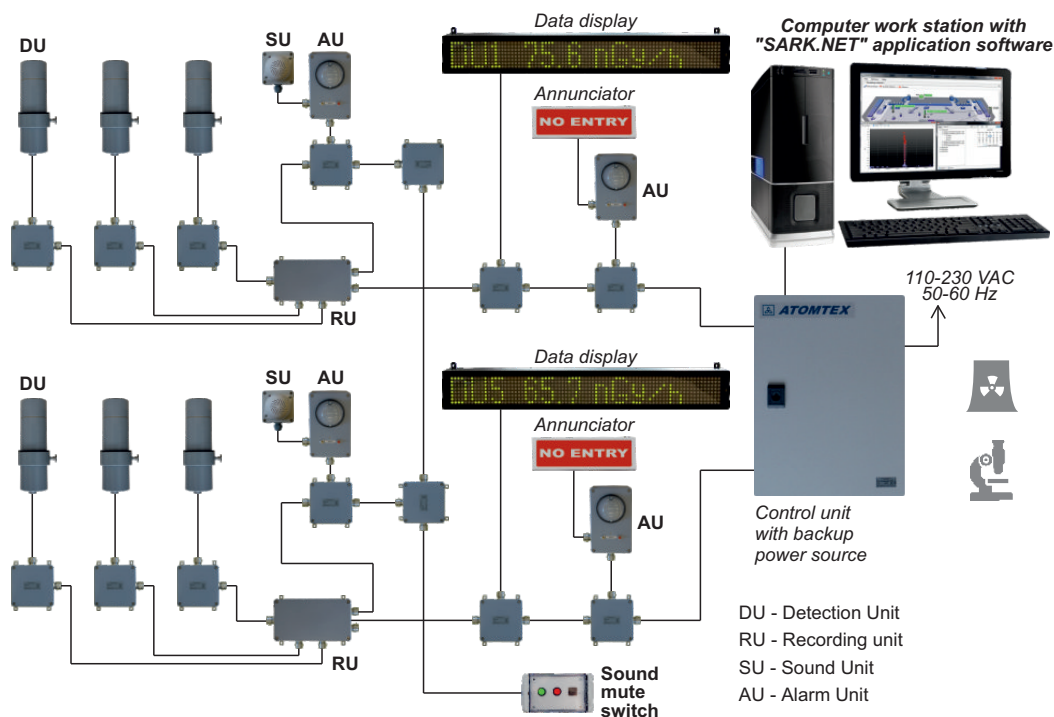

Sample functional chart of Alarm system for detection of occurrence of self-sustaining chain reaction

Detection of self-sustaining chain reaction and generation of alarm signals to evacuate personnel from hazardous area.


AT2331 can be combined with AT2327 *Alarm Dosimeter* and a personal computer running "SARK.NET" software to create an alarm system for detection of occurrence of self-sustaining chain reaction.

- Detection of self-sustaining chain reaction in full range of its characteristics
- High reliability
- Self-monitoring of component parts
- Backup power source
- Logging measurement results into non-volatile memory of alarm dosimeter
- Integration into external security systems

| | | |
|---|-------------------------------------|--|
| Scintillation detector | | Plastic Ø10x5 mm |
| Minimum duration of a registered self-sustaining chain reaction | | 1 ms |
| Measurement range: - Absorbed dose rate - Absorbed dose | | 0.1 µGy/h – 1 Gy/h 0.05 µGy – 10 Gy |
| Energy range | | 60 keV – 3 MeV |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | | ±35% |
| Selectable dose rate threshold range | | 1 µGy/h – 1 Gy/h |
| Time interval from the moment of response to the moment when the rated alarm sound level is reached | | ≤0.5 s |
| Alarm sound level at 1-meter distance | | 100 dB |
| Number of measurement channels | | Up to 32 |
| Continuous battery operation time | | ≥6 h |
| Protection class | DU and switches other components | IP57 IP65 |

Design and specifications are subject to change without notice

Area Monitor for Pulse Radiation

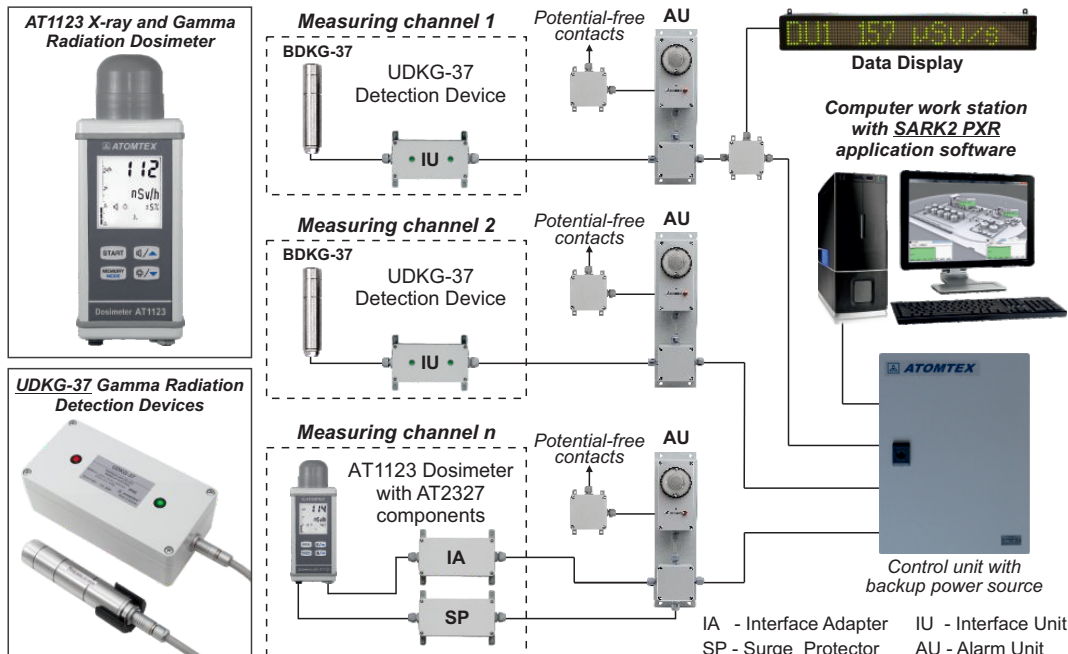

Restricted area beamline radiation control at linear accelerators (LINACs) and other pulse radiation facilities.

Measurement point may be either in the operator's room or directly at the LINAC or facility location.




- Logging of dose rate levels and threshold exceeding events
- Software for displaying current radiation environment in controlled area on PC screen
- Backup power source for autonomous operation up to 6 hours
- Fault diagnostics

| Measuring channel | UDKG-37 | AT1123 |
|--|---|--|
| Detector | Silicon semiconductor detector; Geiger-Muller counter tube | Scintillation tissue-equivalent plastic Ø30x15 mm |
| Measurement range of average ambient dose equivalent rate of pulse radiation | 30 $\mu\text{Sv/s}$ – 0.3 Sv/s (100 mSv/h – 1000 Sv/h) (pulse repetition rate is not less than 20 cps, duration not less than 1 μs) | 30 $\mu\text{Sv/s}$ – 3 mSv/s (0.1 $\mu\text{Sv/h}$ – 10 Sv/h) (pulse repetition rate is not less than 10 cps, duration not less than 10 ns) |
| Measurement range of ambient dose equivalent rate of continuous radiation | 1 $\mu\text{Sv/h}$ – 5000 Sv/h | 50 nSv/h – 10 Sv/h |
| Measurement range of ambient dose equivalent | – | 10 nSv – 10 Sv |
| Energy range | 50 keV – 10 MeV | 15 keV – 10 MeV |
| Typical sensitivity to ^{137}Cs gamma radiation | 0.15 cps/($\mu\text{Sv}\cdot\text{h}^{-1}$), for dose rate ≤ 0.1 Sv/h 58 mV/(Sv $\cdot\text{h}^{-1}$), for dose rate > 0.1 Sv/h | 70 cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) |
| Burn-up life | ≥ 50000 Sv | ≥ 100 Sv |
| Number of measurement channels | Up to 32 | |
| Protection class | IP68 (BDKG-37), IP54 (AT1123), IP65 (other components) | |

Design and specifications are subject to change without notice

Spectrometric System for Radiation Monitoring

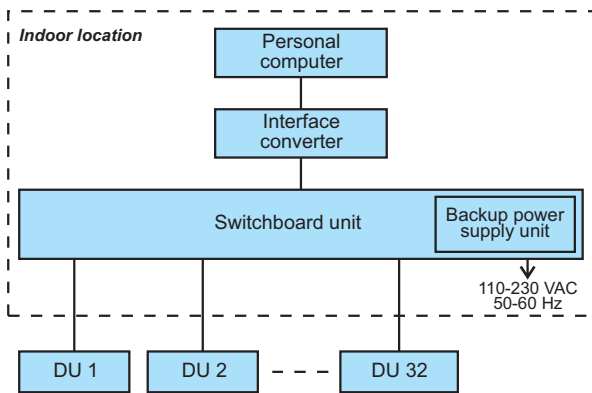

Structural diagram of the system

Spectrometric and dosimetric radiation control of area, facilities, wells and other sites.

- Indication of spectra and dose rate readings by each detection unit (DU) on site plan or terrain map
- Identification of source radionuclide composition
- Energy range expandable to 5 MeV
- Hermetically sealed construction (IP68)
- Backup power source



| | |
|--|--|
| Number of detection units (DUs) in the system | 1 – 32 |
| Maximum distance of communication line between DUs and the PC | 1000 m |
| Maximum distance of communication line between switchboard unit and PC | 100 m |
| Identified radionuclides | Medical, industrial, natural (The library content can be modified on request) |
| Continuous battery operation time | ≥6 h |
| PC interface | USB / Ethernet / Bluetooth (via interface adapter) |

| Detection Unit | BDKG-201M | BDKG-203M | BDKG-205M | BDKG-211M | BDKG-219M |
|--|--|----------------------|----------------------|-----------------------|-----------------------|
| Scintillation detector | NaI(Tl) Ø25x16 mm | NaI(Tl) Ø25x40 mm | NaI(Tl) Ø40x40 mm | NaI(Tl) Ø63x63 mm | NaI(Tl) Ø63x160 mm |
| Energy range | 20 keV – 3 MeV | | | | |
| Measurement range of ambient dose equivalent rate | 50 nSv/h – 1 mSv/h | 30 nSv/h – 500 µSv/h | 30 nSv/h – 300 µSv/h | 30 nSv/h – 120 µSv/h | 30 nSv/h – 50 µSv/h |
| | Limits of tolerable intrinsic relative error: ±20% | | | | |
| Typical sensitivity to gamma radiation, cps/(µSv·h ⁻¹) | ²⁴¹ Am 1400 ¹³⁷ Cs 165 ⁶⁰ Co 80 | 3600 400 190 | 5400 800 420 | 13900 2450 1300 | 37000 6000 2500 |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | ±15% (50 keV – 3 MeV) | | | | |
| Typical resolution at 662 keV (¹³⁷ Cs) | 8.5% | 8% | 7.5% | 7.5% | 8% |
| Protection class | IP68 (Fresh water measurement at depths up to 50 m. Holds hydrostatic pressure up to 5 atm or 0.6 MPa) | | | | |
| Interface | RS485 | | | | |
| Operation temperature range | -35...+55°C | -35...+55°C | -35...+55°C | -35...+55°C | -35...+55°C |
| Dimensions, weight | Ø63x313 mm, 1 kg | Ø63x333 mm, 1 kg | Ø63x333 mm, 1 kg | Ø90x350 mm, 2 kg | Ø90x430 mm, 3.3 kg |
| Image | | | | | |

Design and specifications are subject to change without notice

AT920B, AT920P Pedestrian Radiation Monitors

Detection of gamma radiation sources in a stream of people crossing borders of controlled facilities.

- Rapid accommodation to changes in radiation background
- Sound and light alarm
- Multiple pedestrian radiation monitors (up to 32) can be joined into a network controlled by dedicated software running on a PC
- Mobility and rapid deployment for passage control
- High reliability and self-check function
- Backup power source



| | | AT920B | AT920P |
|--|---|--|-------------------------------|
| Scintillation detector | | Nal(Tl) Ø63x160 mm | Plastic Ø70x150 mm |
| Energy range | | 50 keV – 3 MeV | 20 keV – 3 MeV |
| Typical sensitivity, cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | ^{241}Am ^{137}Cs ^{60}Co | 30650 4900 3140 | 10000 3200 1600 |
| Minimal detectable gamma radiation dose rate level above background value 0.1 $\mu\text{Sv/h}$ in a period not longer than 2 s | | 0.03 $\mu\text{Sv/h}$ | 0.04 $\mu\text{Sv/h}$ |
| Detection threshold for unshielded source at 1 m height under natural radiation background conditions not more than 0.1 $\mu\text{Sv/h}$ | ^{241}Am ^{137}Cs ^{60}Co | 1 MBq 320 kBq 130 kBq | 2.3 MBq 370 kBq 190 kBq |
| | (Distance to source 1 m, source travel speed 5 km/h, probability of source detection 80 % under confidence level $P=0.95$) | | |
| False alarm rate | | ≤ 1 for 8 h of continuous operation | |
| PC interface | | RS485 | |
| Continuous battery operation time | | ≥ 6 h | |
| Protection class | | IP54 | |
| Overall dimensions | | Ø350x1220 mm | |
| Weight | | 14.5 kg | 13.5 kg |



AT930 Pedestrian Radiation Monitor



Detection of gamma radiation sources in a stream of people crossing borders of secure facilities.

- Rapid accommodation to radiation background change
- Sound and light alarm
- Continuous and occasional radiation monitoring
- Mobility and capability to create safety lanes
- High integrity and self-checking function
- Backup power source



Conformance to international standard **IEC 62244:2006**

Radiation protection instrumentation - Installed radiation monitors for the detection of radioactive and special nuclear materials at national borders

| | | |
|---|---|-------------------------|
| Detector | Scintillation plastic 1000x100x50 mm | |
| Energy range | 60 keV – 3 MeV | |
| Typical sensitivity, cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co | 60000 31000 16500 |
| False alarm rate | ≤1 per 1000 passings | |
| PC interface | RS485 | |
| Protection class | IP54 | |
| Overall dimensions | 1610x450x300 mm when anchored to the floor (An additional base of 930x760 mm size is included into the delivery set for operation without anchoring) | |
| Weight | 70 kg (83 kg with additional base) | |



Detection threshold for unshielded source at 1 m height under natural radiation background conditions not more than 0.1 $\mu\text{Sv/h}$

(Distance to source 1 m, source travel speed 5 km/h, probability of source detection 80 % under confidence level $P=0.95$)

| | |
|-------------------|---------|
| ²⁴¹ Am | 530 kBq |
| ¹³⁷ Cs | 70 kBq |
| ⁶⁰ Co | 35 kBq |
| ^{99m} Tc | 180 kBq |
| ¹³³ Ba | 75 kBq |
| ¹³¹ I | 50 kBq |

Minimum detectable amount of radioactive materials at 1 m height under natural radiation background conditions not more than 0.1 $\mu\text{Sv/h}$

(Distance to source 1 m, source travel speed 5 km/h, probability of source detection 95% under confidence level $P=0.95$)

| | |
|-------------------|-------|
| ²³⁵ U | 15 g |
| ²³⁹ Pu | 1.2 g |

Pedestrian Radiation Monitors (based on AT2327 Alarm Dosimeter)



Consisting of:
BDKG-19 (BDKG-35)
and
BDKN-01 (BDKN-05)



Consisting of:
BD RM-05 and BDKN-05

Detection of gamma and neutron radiation sources in a stream of people crossing borders of controlled facilities.

- Rapid accommodation to changes in radiation background
- Sound and light alarm
- Multiple pedestrian radiation monitors (up to 32) can be joined into a network controlled by dedicated software running on a PC
- High reliability and self-check function
- Backup power source

| | |
|-----------------------------------|------------------------------------|
| False alarm rate | ≤1 for 8 h of continuous operation |
| PC interface | RS485 |
| Continuous battery operation time | ≥6 h |
| Protection class | IP65 |
| Overall dimensions, weight | depending on configuration |

| Gamma radiation detection unit (DU) | | | BDKG-19 | BDKG-35 | BD RM-05 |
|--|------|--|-------------------------------|--------------------------------|------------------------------|
| Scintillation detector | | | Nal(Tl) Ø63x160 mm | Plastic Ø70x150 mm | Plastic 1000x100x50 mm |
| Energy range | | | 50 keV – 3 MeV | 20 keV – 3 MeV | 50 keV – 3 MeV |
| Typical sensitivity, cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | | ^{241}Am ^{137}Cs ^{60}Co | 32500 4900 2800 | 10000 3600 2300 | 60000 31500 16500 |
| Minimal detectable gamma radiation dose rate level above background value 0.1 $\mu\text{Sv/h}$ in a period not longer than 2 s | | | 0.03 $\mu\text{Sv/h}$ | 0.04 $\mu\text{Sv/h}$ | 0.01 $\mu\text{Sv/h}$ |
| Detection threshold for unshielded source at 1 m height under natural radiation background conditions not more than 0.1 $\mu\text{Sv/h}$ | 1 DU | ^{241}Am ^{137}Cs ^{60}Co | 430 kBq 220 kBq 100 kBq | 1180 kBq 230 kBq 100 kBq | 800 kBq 110 kBq 60 kBq |
| | 2 DU | ^{241}Am ^{137}Cs ^{60}Co | 320 kBq 160 kBq 70 kBq | 860 kBq 170 kBq 70 kBq | 580 kBq 80 kBq 40 kBq |
| (Distance to source 1 m, source travel speed 5 km/h, probability of source detection 80 % under confidence level $P=0.95$) | | | | | |

| Neutron radiation detection unit (DU) | | | BDKN-01 | BDKN-05 |
|---|------|-------------------|--|--|
| Detector | | | He-3 proportional counter in polyethylene moderator | Two He-3 proportional counters in polyethylene moderator |
| Energy range | | | 0.025 eV – 14 MeV | 0.025 eV – 14 MeV |
| Typical sensitivity to source radiation at the distance of 1 m | | ²⁵² Cf | 1.3 cps/(neutron·s ⁻¹ ·cm ⁻²) | 20 cps/(neutron·s ⁻¹ ·cm ⁻²) |
| Source detection threshold at 1 m height | 1 DU | ²⁵² Cf | 2.2·10 ⁵ neutron/s | 2.3·10 ⁴ neutron/s |
| | 2 DU | ²⁵² Cf | – | 1.6·10 ⁴ neutron/s |
| (Distance to source 1 m, source travel speed 5 km/h, probability of source detection 80% under confidence level P=0.95) | | | | |

Design and specifications are subject to change without notice

Vehicle Radiation Monitors (based on AT2327 Alarm Dosimeter)



Version of the vehicle radiation monitor with the following configuration:
BDKG-19 (2 units), BDKN-05 (2 units)



Version of the vehicle radiation monitor with the following configuration:
BDRM-05 (4 units), BDKN-05 (4 units)




Version of the vehicle radiation monitor with the following configuration:
BDRM-05 (8 units), BDKN-05 (8 units)

Detection of gamma and neutron radiation sources in vehicles crossing access control points.

- Modular system design
- Automatic adjustment of set threshold levels according to changes in natural radiation background
- High reliability and self-check function
- Backup power source
- Automatic data logging
- Optional CCTV connectivity



| | |
|-----------------------------------|----------------------------|
| Detection time per one vehicle | ≤20 s |
| False alarm rate | ≤1 per 1000 crossings |
| Continuous battery operation time | ≥6 h |
| Protection class | IP65 |
| Overall dimensions, weight | depending on configuration |

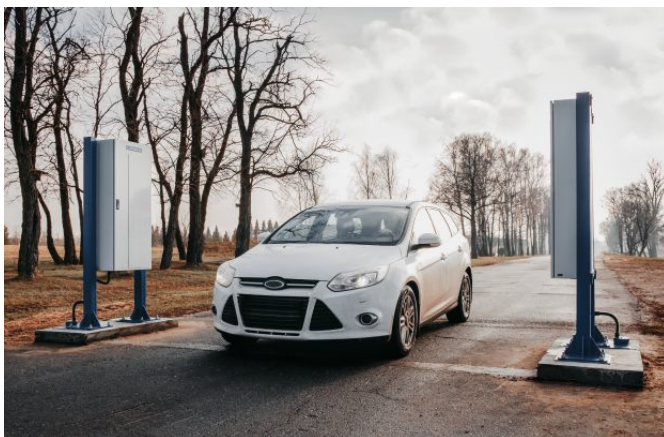

Pedestrian and Vehicle Radiation Monitors

Vehicle Radiation Monitors (based on AT2327 Alarm Dosimeter)





| Gamma radiation detection unit (DU) | | BDKG-19 | BDKG-35 | BDRM-05 |
|--|--|-----------------------|-----------------------|---------------------------|
| Scintillation detector | | Nal(Tl) Ø63x160 mm | Plastic Ø70x150 mm | Plastic 1000x100x50 mm |
| Energy range | | 50 keV – 3 MeV | 20 keV – 3 MeV | 50 keV – 3 MeV |
| Typical sensitivity, cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co | 32500 4900 2800 | 10000 3600 2300 | 60000 31500 15000 |
| Minimal detectable gamma radiation dose rate level above background value 0.1 $\mu\text{Sv/h}$ in a period not longer than 2 s | | 0.03 $\mu\text{Sv/h}$ | 0.04 $\mu\text{Sv/h}$ | 0.01 $\mu\text{Sv/h}$ |

| Neutron radiation detection unit (DU) | | BDKN-05 | |
|---|-------------------|---|--|
| Detector | | Two He-3 proportional counters in polyethylene moderator | |
| Energy range | | 0.025 eV – 14 MeV | |
| Typical sensitivity to source radiation at the distance of 1 m | ²⁵² Cf | 20 cps/(neutron·s ⁻¹ ·cm ⁻²) | |



Detection threshold for unshielded source

under natural radiation background conditions not more than 0.1 $\mu\text{Sv/h}$
(Probability of source detection 80% under confidence level $P=0.95$)

Road vehicles. Travel speed 8 km/h

| | DU configuration (location and number) | BDKG-19 | BDKG-35 | BDRM-05 | BDKN-05 |
|--|---|---|---|--|--|
| Control zone width – 3 m, height – 2 m |  | 1100 kBq [²⁴¹ Am] 470 kBq [¹³⁷ Cs] 220 kBq [⁶⁰ Co] | 2850 kBq [²⁴¹ Am] 550 kBq [¹³⁷ Cs] 230 kBq [⁶⁰ Co] | 1800 kBq [²⁴¹ Am] 280 kBq [¹³⁷ Cs] 120 kBq [⁶⁰ Co] | 4.1·10 ⁴ neutron/s [²⁵² Cf] |
| |  | 770 kBq [²⁴¹ Am] 320 kBq [¹³⁷ Cs] 160 kBq [⁶⁰ Co] | 1940 kBq [²⁴¹ Am] 370 kBq [¹³⁷ Cs] 150 kBq [⁶⁰ Co] | 1200 kBq [²⁴¹ Am] 160 kBq [¹³⁷ Cs] 90 kBq [⁶⁰ Co] | 2.5·10 ⁴ neutron/s [²⁵² Cf] |
| Control zone width – 6 m, height – 4.5 m |  | 2700 kBq [²⁴¹ Am] 1190 kBq [¹³⁷ Cs] 540 kBq [⁶⁰ Co] | 6900 kBq [²⁴¹ Am] 1350 kBq [¹³⁷ Cs] 550 kBq [⁶⁰ Co] | 4400 kBq [²⁴¹ Am] 550 kBq [¹³⁷ Cs] 270 kBq [⁶⁰ Co] | 4.4·10 ⁴ neutron/s [²⁵² Cf] |
| |  | 1860 kBq [²⁴¹ Am] 800 kBq [¹³⁷ Cs] 370 kBq [⁶⁰ Co] | 4950 kBq [²⁴¹ Am] 890 kBq [¹³⁷ Cs] 370 kBq [⁶⁰ Co] | 3000 kBq [²⁴¹ Am] 400 kBq [¹³⁷ Cs] 200 kBq [⁶⁰ Co] | 2.6·10 ⁴ neutron/s [²⁵² Cf] |

Railway vehicles. Travel speed 20 km/h

| | DU configuration (location and number) | BDKG-19 | BDKG-35 | BDRM-05 | BDKN-05 |
|--|---|---------|---------|--|--|
| Control zone width – 6 m, height – 4.5 m |  | – | – | 6900 kBq [²⁴¹ Am] 880 kBq [¹³⁷ Cs] 470 kBq [⁶⁰ Co] | 8.0·10 ⁴ neutron/s [²⁵² Cf] |
| |  | – | – | 5200 kBq [²⁴¹ Am] 650 kBq [¹³⁷ Cs] 310 kBq [⁶⁰ Co] | 4.9·10 ⁴ neutron/s [²⁵² Cf] |

Design and specifications are subject to change without notice

AT6110 Radiation Portal Monitor (rapid deployable)



Monitor
1630x460x190 mm, 45 kg

Detection of gamma and neutron radiation sources in vehicles, cargo and pedestrian traffic.

- Rapid deployment
- High sensitivity
- Categorization of radiation sources into natural and artificial
- Up to 20 h of operation time on built-in batteries
- Storage and operation in rugged cases
- Severe operating conditions



**Case with frames (x2)
and accessories**
1550x550x465 mm, 65 kg

*Rugged 10"
tablet PC
for control and
indication*



Pedestrian and Vehicle Radiation Monitors

AT6110 Portal Radiation Monitor (rapid deployable)

| | |
|--|--|
| Monitor configuration | Gamma channel: 1 x BDRM-05 Neutron channel: 2 x BDKN-05 |
| Total number of monitors in the system | Up to 8 |
| Time of continuous operation | ~ 20 h |
| Monitors power supply | Built-in rechargeable battery pack |
| Protection class | IP55 |
| Dimensions and weight of monitor attached to frame (in operating position) | 2090x1025x955 mm, 78 kg |





| Gamma radiation detection units | | BDRM-05 |
|---|--|--|
| Scintillation detector | | Plastic, 1000x100x50 mm |
| Energy range | | 50 keV – 3 MeV |
| Typical sensitivity to source radiation | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co | 60000 cps/(μSv·h ⁻¹) 32000 cps/(μSv·h ⁻¹) 17000 cps/(μSv·h ⁻¹) |

| Neutron radiation detection units | | BDKN-05 |
|--|-------------------|--|
| Detector | | Two He-3 proportional counters in polyethylene moderator |
| Energy range | | 0.025 eV – 14 MeV |
| Typical sensitivity to source radiation at the distance of 1 m | ²⁵² Cf | 20 cps/(neutron·s ⁻¹ ·cm ⁻²) |


Detection threshold for unshielded source

under natural radiation background conditions not more than 0.1 μSv/h
(Probability of source detection 80% under confidence level P=0.95)

Road vehicles. Travel speed 8 km/h

| | Monitors configuration (location and number) | Gamma channel | | Neutron channel |
|--|---|--|--|---|
| | | Detection | Categorization | |
| Control zone width – 3 m, height – 2 m |  | 940 kBq [²⁴¹ Am] 130 kBq [¹³⁷ Cs] 70 kBq [⁶⁰ Co] | 1100 kBq [²⁴¹ Am] 310 kBq [¹³⁷ Cs] 330 kBq [⁶⁰ Co] | 2.1·10 ⁴ neutron/s [²⁵² Cf] |
| |  | 690 kBq [²⁴¹ Am] 100 kBq [¹³⁷ Cs] 50 kBq [⁶⁰ Co] | 800 kBq [²⁴¹ Am] 240 kBq [¹³⁷ Cs] 250 kBq [⁶⁰ Co] | 1.2·10 ⁴ neutron/s [²⁵² Cf] |
| Control zone width – 6 m, height – 4.5 m |  | 2140 kBq [²⁴¹ Am] 290 kBq [¹³⁷ Cs] 150 kBq [⁶⁰ Co] | 2500 kBq [²⁴¹ Am] 690 kBq [¹³⁷ Cs] 710 kBq [⁶⁰ Co] | 2.2·10 ⁴ neutron/s [²⁵² Cf] |
| |  | 1570 kBq [²⁴¹ Am] 210 kBq [¹³⁷ Cs] 110 kBq [⁶⁰ Co] | 1900 kBq [²⁴¹ Am] 500 kBq [¹³⁷ Cs] 520 kBq [⁶⁰ Co] | 1.4·10 ⁴ neutron/s [²⁵² Cf] |

AT110, AT130 Gamma Beam Irradiators with Calibration Bench

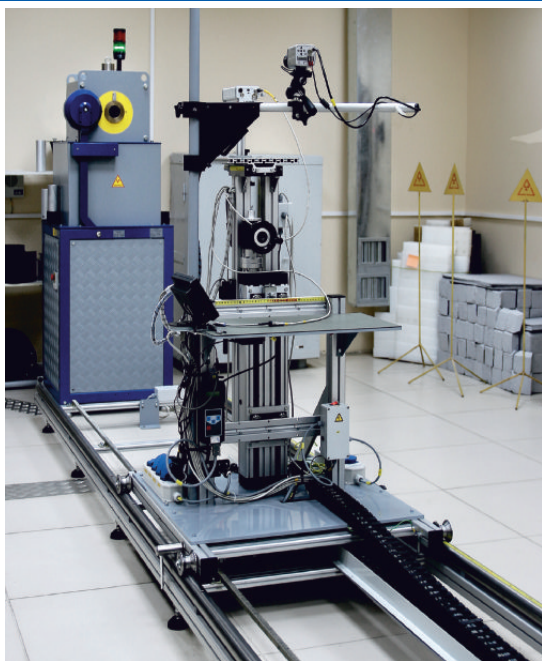

Reproduction and transfer of air kerma, exposure dose, ambient dose equivalent, personal dose equivalent units and their respective rates into working standards and measurement instruments during verification, calibration and test procedures.

- Irradiator with collimator of typical design
- Rotary drum magazine for sources in tungsten and lead protection
- Software control of source movement and moving platform positioning
- Alarm and interlock systems, area monitors
- Control by operator panel or personal computer with automatic calibration capability



| | AT110 | AT130 |
|---|---|--|
| Gamma radiation sources, maximum activity | ^{137}Cs : $1.3 \cdot 10^{12}$ Bq (35 Ci) | ^{137}Cs : $9.6 \cdot 10^{13}$ Bq (2600 Ci) ^{60}Co : $7.2 \cdot 10^8$ Bq (0.2 Ci) ^{241}Am : $1.6 \cdot 10^{10}$ Bq (0.4 Ci) |
| Number of sources | up to 5 | up to 6 |
| Ranges: - Air kerma rate - Exposure dose rate - Ambient and personal dose equivalent rates | 0.25 $\mu\text{Gy/h}$ – 350 mGy/h 30 $\mu\text{R/h}$ – 40 R/h 0.30 $\mu\text{Sv/h}$ – 420 mSv/h | 0.36 $\mu\text{Gy/h}$ – 50 Gy/h 40 $\mu\text{R/h}$ – 5400 R/h 0.43 $\mu\text{Sv/h}$ – 58 Sv/h |
| Intrinsic relative error for certification as a working standard of 1-st category (2-nd category) | $\pm 2.5\%$ ($\pm 5\%$) for air kerma rate and exposure dose rate $\pm 4.5\%$ ($\pm 7\%$) for ambient and personal dose equivalent rates | |

Actual values of range limits and errors are determined by calibration
Design and specifications are subject to change without notice

AT140 Neutron Calibration Facility



Reproduction and transfer of neutron flux density, ambient dose equivalent rate and personal dose equivalent rate units of neutron radiation during calibration, verification and testing of neutron radiation monitors and dosimeters.

| | |
|---|--|
| Source of neutrons, peak neutron flux | $^{238}\text{Pu-Be}$: $5 \cdot 10^7$ neutron/s ^{252}Cf : $5 \cdot 10^8$ neutron/s |
| Number of sources | up to 3 |
| Ranges: - Fast neutron flux density - Slow neutron flux density - Ambient and personal dose equivalent rates | $2.5 - 3.5 \cdot 10^3$ neutron/(s·cm ²) $1 - 1.4 \cdot 10^3$ neutron/(s·cm ²) $3.5 - 4.0 \cdot 10^3$ μSv/h |
| Intrinsic relative error: - Neutron flux density - Ambient and personal dose equivalent rates | ±5% ±7% |

- Fast and slow neutrons field in collimated beam
- Fast neutron field in "open" geometry using shielding cone according to ISO 8529-2
- Drum magazine for sources in polyethylene and concrete protection at the depth of 1 m
- Software control of source movement and moving platform positioning
- Alarm and interlock systems, area monitors
- Control by operator panel or personal computer with automatic calibration capability



*Actual values of range limits and errors are determined by calibration
Design and specifications are subject to change without notice*

Combined use of AT130 and AT140 facilities



Automated calibration facilities are the next generation equipment providing high quality metrology support of radiation monitoring instruments, top-level radiation safety and durability.

AT130 and AT140
Control area
(Operator's room)



AT300, AT300/1, AT300/2 X-ray Calibration Systems



Storage and transfer of air kerma, ambient, individual and directional dose equivalents and dose equivalent rates of X-ray radiation into working standards and measurement instruments.




- High-stable ISOVOLT X-ray units with metal-ceramic tubes
- Field shaper with radiation quality according to GOST 8.087, ISO 4037, IEC 61267, etc.
- Interchangeable disks with 11 sockets for filters; 3 interchangeable diaphragms
- Additional filters with thickness up to 50 mm
- Tungsten safety shutter attenuates the beam by a factor of 1000 and has operating time of less than 0.1 s
- The camera-monitor assembly and spectrometric unit control the availability and stability of radiation output
- The system for 3-axes positioning in radiation beam
- Laser tools for detector alignment
- Video surveillance system for measurements
- Alarm and interlock systems, area monitors
- Control system based on PC and operator panels

| | AT300 | AT300/1 | AT300/2 |
|---|--|---|---|
| Type of X-ray unit | ISOVOLT Titan E 320 | ISOVOLT Titan E 225 | ISOVOLT Titan E 160 |
| Anode voltage range | 5 – 320 kV | 5 – 225 kV | 5 – 160 kV |
| Filtration of X-ray tube | <4 mm Be | <1 mm Be | <1 mm Be |
| Air kerma rate range (Air kerma) | $2 \cdot 10^{-8} - 2 \cdot 10^{-2}$ Gy/s ($2.8 \cdot 10^{-7} - 20$ Gy) | $2 \cdot 10^{-8} - 1.5 \cdot 10^{-2}$ Gy/s ($2.5 \cdot 10^{-7} - 15$ Gy) | $2 \cdot 10^{-8} - 1.5 \cdot 10^{-2}$ Gy/s ($3.5 \cdot 10^{-7} - 15$ Gy) |
| Ambient, individual and directional dose equivalent rate (Ambient, individual and directional dose equivalent) | $2.7 \cdot 10^{-8} - 3.2 \cdot 10^{-3}$ Sv/s ($3.3 \cdot 10^{-7} - 3.2$ Sv) | $2.7 \cdot 10^{-8} - 3.2 \cdot 10^{-3}$ Sv/s ($3.3 \cdot 10^{-7} - 3.2$ Sv) | $5.3 \cdot 10^{-8} - 3.2 \cdot 10^{-3}$ Sv/s ($5.2 \cdot 10^{-7} - 3.2$ Sv) |
| Intrinsic relative error <i>for certification as a working standard of 1-st category</i> | $\pm 3\%$ for air kerma and air kerma rate $\pm 5\%$ for ambient, individual and directional dose equivalent and their rates | | |

Actual values of range limits and errors are determined by calibration
Design and specifications are subject to change without notice

AT200 Beta Calibration Facility

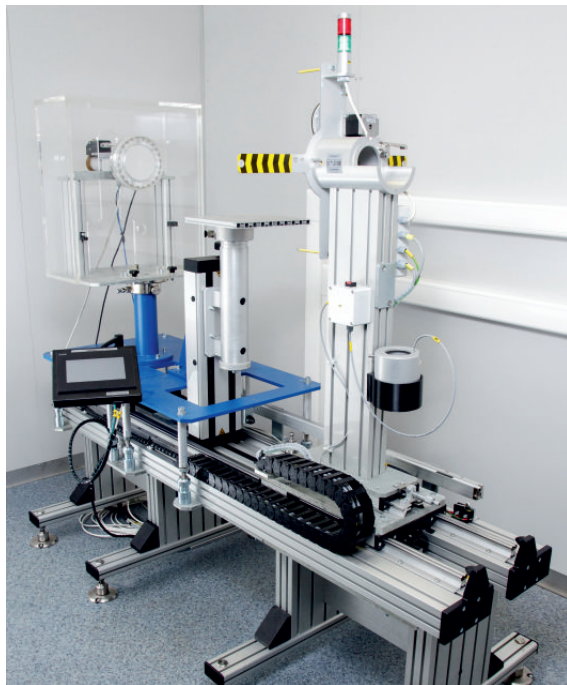

Transfer of absorbed dose, directional and personal dose equivalents and dose equivalent rates of beta radiation into working standards, dosimeters for absorbed dose measurement into tissues and personal dosimeters of beta radiation during their calibration and verification.



- Sealed radionuclide sources of beta radiation $^{90}\text{Sr}+^{90}\text{Y}$ (BIS-50, 22 GBq), ^{85}Kr (KAC.D3, 15 GBq) and ^{147}Pm (BIP-50, 10 GBq) can be used
- The shape of reference field around sources can be changed by movable irradiator unit using smoothing filters
- Source holders with a shutter and safety shields
- Calibrated rods and a laser device for centering and digitization
- Video surveillance system for measurements
- Can be used as part of an automated beta-radiation extrapolation chamber for simulation of absorbed dose (absorbed dose rate) of beta radiation in tissue
- Measurement of ionization current values starting from 1 fA using extrapolation chamber and precision electrometer
- Software for facility control, performing calibration and for calculations
- Alarm and interlock system, photon radiation monitoring system in measurement and control rooms



| | | |
|--|-------------------------|---|
| The range of beta radiation absorbed dose rate $D_{\text{r}}(0.07)$ (rated limits) | | $10 - 5.5 \cdot 10^3 \text{ } \mu\text{Gy/s}$ |
| Source positioning error | | 0.1 mm |
| Travel range of irradiator unit in measurement geometry: | "Dosimeters" | 100 – 500 mm |
| | "Extrapolation Chamber" | |
| Intrinsic error for absorbed dose rate of beta radiation | | $\pm 5\%$ |
| Diameter of irradiator exit window | | 55 mm |
| Height of radiation beam axis | | 1300 mm |

*Actual values of range limits and errors are determined by calibration
Design and specifications are subject to change without notice*

Equipment for Neutron Spectrometry

AT1117M Radiation Monitor with BDKN-06 Detection Unit and a set of spherical moderators

Measurement of neutron radiation characteristics to reconstruct the energy distribution of neutron flux density.



PU4 Processing Unit

Obtained energy distribution of neutron flux density is used to calculate such values as:

- Integral neutron flux density
- Average energy of neutron radiation by spectrum
- Average energy of neutron radiation by dose
- Dose equivalent per unit flux density
- Dose equivalent
- Effective dose

- Ready-to-use measurement procedures
- Advanced set of spherical polyethylene moderators is available with the following diameters: 3.5"; 4.5"; 5"; 7"; 9"; 9.5"



| | |
|---|--|
| Detector | ^3He proportional counter |
| Energy range | 0.025 eV – 20 MeV |
| Measurement range of neutron count rate | $0.01 - 5 \cdot 10^4$ cps |
| Limits of tolerable intrinsic relative error (P=0.95) for neutron measurement | $\pm 10\%$ |
| Detection range of neutron flux density | $1 \cdot 10^{-16} - 5 \cdot 10^{12}$ neutron/($\text{s} \cdot \text{cm}^2 \cdot \text{MeV}$) |
| Typical neutron sensitivity | 1 cps/(neutron $\cdot \text{s}^{-1} \cdot \text{cm}^2$) [Pu-Be] |
| Relative sensitivity due to the incidence angle of neutrons | up to -25% |
| Protection class | IP64 |
| Overall dimensions, weight | 550x254x254 mm, 10 kg (with Ø254 mm (Ø10") spherical moderator without tripod) |

Part of robot devices for land, aircraft and marine applications




Wide range of detection units:

- For X-ray, gamma, alpha, beta and neutron radiation
- Of dosimetric, spectrometric and radiometric type
- For operating temperatures from -40 to $+70^{\circ}\text{C}$
- With USB/RS232/RS485/Bluetooth interfaces
- Capability to import all measurement data to a PC for further expert software-assisted processing



Courtesy of CERN

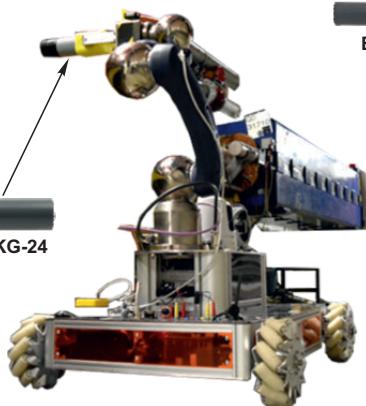









Courtesy of CERN



For specifications of the detection units see pages 47-51 and pages 11-13 (Detection units in the complete set of AT1117M Radiation monitor)

Dosimetric Gamma Radiation Detection Units




| Detection Unit | | BDKG-04 | BDKG-24 | BDKG-25 | BDKG-30 |
|--|--|---|---|---|--|
| Scintillation detector | | Tissue-equivalent plastic, Ø30x15 mm | Tissue-equivalent plastic, Ø50x40 mm | Scintillation plastic, Ø10x5 mm | Tissue-equivalent plastic, Ø50x40 mm |
| Energy range | | 15 keV – 10 MeV | 25 keV – 10 MeV | 60 keV – 3 MeV | 50 keV – 10 MeV |
| Measurement range of ambient dose equivalent rate | | 50 nSv/h – 10 Sv/h | 30 nSv/h – 1 Sv/h | – | – |
| Measurement range of air kerma rate | | – | – | 0.1 µGy/h – 1 Gy/h | 30 nGy/h – 1 Gy/h |
| Limits of tolerable intrinsic relative error | | ±20% | ±20% | ±20% | ±20% |
| Typical sensitivity to gamma radiation, cps/(µSv·h ⁻¹) | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co | 370 70 40 | 3200 530 270 | cps/(µGy·h ⁻¹) 75 3.5 2 | cps/(µGy·h ⁻¹) 2800 600 290 |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | | ±25% (15 keV - 3 MeV) ±40% (3 - 10 MeV) | ±25% (25 keV - 3 MeV) ±40% (3 - 10 MeV) | ±35% | ±25% (50 keV - 3 MeV) ±40% (3 - 10 MeV) |
| Protection class | | IP64 | IP64 | IP57 | IP64 |
| Interface | | RS232 | RS232 | RS485 | RS232 |
| Operation temperature range | | -50...+50°C | -50...+50°C | -40...+50°C | -50...+50°C |
| Dimensions, weight | | Ø60x200 mm, 0.46 kg | Ø60x205 mm, 0.5 kg | Ø60x210 mm, 0.6 kg | Ø60x207 mm, 0.6 kg |
| Image | |  |  |  |  |




| Detection Unit | | BDKG-32 | BDKG-35 | BDKG-36 | BDKG-38 |
|--|--|---|---|---|--|
| Scintillation detector | | Tissue-equivalent plastic, Ø70x80 mm | Plastic, Ø70x150 mm | Tissue-equivalent plastic, Ø89x89 mm | Tissue-equivalent plastic, Ø89x89 mm |
| Energy range | | 40 keV – 10 MeV | 20 keV – 10 MeV | 40 keV – 10 MeV | 40 keV – 10 MeV |
| Measurement range of ambient dose equivalent rate | | 30 nSv/h – 500 mSv/h | Count rate indication range: 0 – 1.5·10 ⁵ s ⁻¹ | 30 nSv/h – 200 mSv/h | – |
| Measurement range of air kerma rate | | – | | – | 30 nGy/h – 200 mGy/h |
| Limits of tolerable intrinsic relative error | | ±20% | | ±10% | ±10% |
| Typical sensitivity to gamma radiation, cps/(µSv·h ⁻¹) | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co | 8300 1660 850 | 11500 3300 1700 | 10500 2600 1450 | cps/(µGy·h ⁻¹) 12800 3000 1600 |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | | ±25%(40keV-3MeV) ±40%(3-10MeV) | – | ±30%(40-60 keV) ±15%(60keV-3MeV) ±20%(3-10MeV) | ±30%(40-60keV) ±15%(60keV-3MeV) ±20%(3-10MeV) |
| Protection class | | IP64 | IP64 | IP64 | IP64 |
| Interface | | RS232 | RS232 | RS232 | RS232 |
| Operation temperature range | | -50...+50°C | -40...+50°C | -50...+50°C | -50...+50°C |
| Dimensions, weight | | Ø80x245 mm, 0.78 kg | Ø80x320 mm, 1.2 kg | Ø93x250 mm, 1.2 kg | Ø93x250 mm, 1.2 kg |
| Image | |  |  |  |  |

Design and specifications are subject to change without notice

Smart Detection Units and Detection Devices




Dosimetric Gamma Radiation Detection Units






| Detection Unit | | BDKG-22 | BDKG-23/1 | BDKG-23 |
|--|--|---|---|--|
| Detector | | Geiger-Mueller counter tube | Two Geiger-Mueller counter tubes | Two Geiger-Mueller counter tubes |
| Energy range | | 60 keV – 3 MeV | 60 keV – 3 MeV | 60 keV – 3 MeV |
| Measurement range of ambient dose equivalent rate | | 0.1 $\mu\text{Sv/h}$ – 10 Sv/h | 0.1 $\mu\text{Sv/h}$ – 100 Sv/h | – |
| Measurement range of air kerma rate | | – | – | 0.1 $\mu\text{Gy/h}$ – 100 Gy/h |
| Limits of tolerable intrinsic relative error | | $\pm 20\%$ | $\pm 20\%$ | $\pm 20\%$ |
| Typical sensitivity to gamma radiation, cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co | 4 4 4 | 4 4 4 | cps/($\mu\text{Gy}\cdot\text{h}^{-1}$) 4.6 4.6 4.6 |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | | -25...+35% | -25...+35% | -25...+35% |
| Protection class | | IP67 | IP67 | IP67 |
| Interface | | RS422 / RS485 | RS422 / RS485 | RS422 / RS485 |
| Operation temperature range | | -40...+70°C | -40...+70°C | -40...+70°C |
| Dimensions, weight | | Ø60x255 mm, 0.5 kg | Ø60x255 mm, 0.55 kg | Ø60x255 mm, 0.55 kg |
| Image | |  |  |  |

| Detection Unit | | BDKG-204 | BDKG-224 | BDKG-230 |
|--|--|---|---|--|
| Scintillation detector | | Tissue-equivalent plastic, Ø30x15 mm | Tissue-equivalent plastic, Ø50x40 mm | Tissue-equivalent plastic, Ø50x40 mm |
| Energy range | | 20 keV – 10 MeV | 40 keV – 10 MeV | 50 keV – 10 MeV |
| Measurement range of ambient dose equivalent rate | | 50 nSv/h – 10 Sv/h | 30 nSv/h – 1 Sv/h | – |
| Measurement range of air kerma rate | | – | – | 30 nGy/h – 1 Gy/h |
| Limits of tolerable intrinsic relative error | | $\pm 20\%$ | $\pm 15\%$ | $\pm 15\%$ |
| Typical sensitivity to gamma radiation, cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co | 370 70 40 | 3200 530 270 | cps/($\mu\text{Gy}\cdot\text{h}^{-1}$) 2800 600 290 |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | | -45%...+35% (20 - 60 keV) $\pm 25\%$ (60 keV - 3 MeV) $\pm 50\%$ (3 - 10 MeV) | $\pm 25\%$ (40 keV - 3 MeV) $\pm 50\%$ (3 - 10 MeV) | $\pm 25\%$ (50 keV - 3 MeV) $\pm 50\%$ (3 - 10 MeV) |
| Protection class | | IP67 | IP66 / IP67 | IP66 / IP67 |
| Interface | | RS485 | RS485 / RS422 | RS485 / RS422 |
| Operation temperature range | | -40...+60°C | -40...+55°C | -40...+55°C |
| Dimensions, weight | | Ø60x210 mm, 0.55 kg | Ø60x250 mm, 0.6 kg | Ø60x250 mm, 0.6 kg |
| Image | |  |  |  |

Design and specifications are subject to change without notice

Spectrometric Gamma Radiation Detection Units



| Detection Unit | BDKG-05M | BDKG-11M | BDKG-19M |
|--|---|---|--|
| Scintillation detector | Nal(Tl), Ø40x40 mm | Nal(Tl), Ø63x63 mm | Nal(Tl), Ø63x160 mm |
| Energy range | 20 keV – 3 MeV | 20 keV – 3 MeV | 20 keV – 3 MeV |
| Measurement range of ambient dose equivalent rate | 30 nSv/h – 300 µSv/h | 30 nSv/h – 150 µSv/h | 30 nSv/h – 50 µSv/h |
| Limits of tolerable intrinsic relative error | ±20% | ±20% | ±20% |
| Typical sensitivity to gamma radiation, cps/(µSv·h ⁻¹) | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co 5400 800 420 | 13500 2200 1200 | 37000 6000 2500 |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | ±15% (50 keV – 3 MeV) | ±15% (50 keV – 3 MeV) | ±15% (50 keV – 3 MeV) |
| Typical energy resolution at 662 keV (¹³⁷ Cs) | 7.5% | 7.5% | 8% |
| Protection class | IP54 | IP54 | IP54 |
| Interface | USB / RS232 / Bluetooth (Interface adapter) | | |
| Operation temperature range | -20...+50°C | -20...+50°C | -20...+50°C |
| Dimensions, weight | Ø60x300 mm, 0.9 kg | Ø78x320 mm, 1.7 kg | Ø78x350 mm, 3 kg |
| Image |  |  |  |

| Detection Unit | BDKG-201M | BDKG-203M | BDKG-205M | BDKG-211M | BDKG-219M |
|--|---|---|---|---|--|
| Scintillation detector | Nal(Tl), Ø25x16 mm | Nal(Tl), Ø25x40 mm | Nal(Tl), Ø40x40 mm | Nal(Tl), Ø63x63 mm | Nal(Tl), Ø63x160 mm |
| Energy range | 20 keV – 3 MeV | 20 keV – 3 MeV | 20 keV – 3 MeV | 20 keV – 3 MeV | 20 keV – 3 MeV |
| Measurement range of ambient dose equivalent rate | 50 nSv/h – 1 mSv/h | 30 nSv/h – 500 µSv/h | 30 nSv/h – 300 µSv/h | 30 nSv/h – 120 µSv/h | 30 nSv/h – 50 µSv/h |
| Limits of tolerable intrinsic relative error | ±20% | ±20% | ±20% | ±20% | ±20% |
| Typical sensitivity to gamma radiation, cps/(µSv·h ⁻¹) | ²⁴¹ Am ¹³⁷ Cs ⁶⁰ Co 1400 165 80 | 3600 400 190 | 5400 800 420 | 13900 2450 1300 | 37000 6000 2500 |
| Energy dependence relative to 662 keV (¹³⁷ Cs) | ±15% (50 keV - 3 MeV) | ±15% (50 keV - 3 MeV) | ±15% (50 keV - 3 MeV) | ±15% (50 keV - 3 MeV) | ±15% (50 keV - 3 MeV) |
| Typical energy resolution at 662 keV (¹³⁷ Cs) | 8.5% | 8% | 7.5% | 7.5% | 8% |
| Protection class | IP68 | IP68 | IP68 | IP68 | IP68 |
| | (Fresh water measurement at depths up to 50 m. Holds hydrostatic pressure up to 5 atm or 0.6 MPa) | | | | |
| Interface | USB / RS232 / RS485 / Bluetooth (Interface adapter) | | | | |
| Operation temperature range | -35...+55°C | -35...+55°C | -35...+55°C | -35...+55°C | -35...+55°C |
| Dimensions, weight | Ø63x313 mm, 1 kg | Ø63x333 mm, 1 kg | Ø63x333 mm, 1 kg | Ø90x350 mm, 2 kg | Ø90x430 mm, 3.3 kg |
| Image |  |  |  |  |  |



Design and specifications are subject to change without notice



Dosimetric Gamma Radiation Detection Devices

Measurement of ambient dose equivalent rate of continuous radiation and average dose rate of pulsed X-ray and gamma radiation in an extremely wide range and under harsh operating conditions.

| Detection Device | | UDKG-37 | UDKG-37/1 |
|---|---------|---|------------------------|
| Components | | BDKG-37 Detection Unit | |
| | | IU-37 Interface Unit | IU-37/1 Interface Unit |
| Detector | | Silicon semiconductor detector; Geiger-Muller counter tube | |
| Energy range | | 50 keV – 10 MeV | |
| Measurement range of ambient dose equivalent rate $\dot{H}^*(10)$ | | 1 $\mu\text{Sv/h}$ – 5000 Sv/h | |
| Limits of tolerable intrinsic relative error | | $\pm 25\%$ (for $\dot{H}^*(10) \leq 10 \mu\text{Sv/h}$) $\pm 15\%$ (for $\dot{H}^*(10) > 10 \mu\text{Sv/h}$) | |
| Measurement range of average pulsed radiation dose rate | | 30 $\mu\text{Sv/s}$ – 0.3 Sv/s (100 mSv/h – 1000 Sv/h) (pulse repetition rate is not less than 20 cps, duration not less than 1 μs) | |
| Limits of tolerable intrinsic relative error | | $\pm 25\%$ (for measurement of average dose rate of pulse radiation) | |
| Typical sensitivity to ^{137}Cs gamma radiation | | 0.15 cps/ $(\mu\text{Sv}\cdot\text{h}^{-1})$ (for $\dot{H}^*(10) \leq 0.1 \text{ Sv/h}$) 58 mV/ $(\text{Sv}\cdot\text{h}^{-1})$ (for $\dot{H}^*(10) > 0.1 \text{ Sv/h}$) | |
| Energy dependence relative to 662 keV (^{137}Cs) | | $\pm 30\%$ | |
| Response time for 10-fold dose rate change | | $\leq 10 \text{ s}$ (for $\dot{H}^*(10) > 10 \mu\text{Sv/h}$) | |
| Burn-up life | | $\geq 50\,000 \text{ Sv}$ | |
| Protection class | BDKG-37 | IP68 (Resistance to static hydraulic pressure up to 400 kPa; water immersion depth up to 40 m) | |
| | IU-37 | IP65 | |
| Interface | | RS485 | RS232 |
| Operation temperature range | | $-40\dots+60^\circ\text{C}$ | |
| Dimensions, weight | BDKG-37 | $\varnothing 30 \times 130 \text{ mm}$, 0.25 kg | |
| | IU-37 | 170x80x55 mm, 0.3 kg | |
| Image | | <div><div><div>IU-37 (IU-37/1)</div></div><div><div>BDKG-37</div></div></div> | |

Neutron Radiation Detection Units

| Detection Unit | | BDKN-01 | BDKN-02 | BDKN-03 | BDKN-04 |
|--|---|---|---------|--|---------|
| Detector: He-3 proportional counter in polyethylene moderator | | One He-3 counter | | One He-3 counter | |
| Energy range | | 0.025 eV – 14 MeV | | 0.025 eV – 14 MeV | |
| Measurement range of ambient dose equivalent rate | | 0.1 $\mu\text{Sv/h}$ – 10 mSv/h [Pu-Be source] | | 0.1 $\mu\text{Sv/h}$ – 10 mSv/h | |
| Typical sensitivity to Pu-Be radiation, (In dose rate measurement mode) | | 0.355 cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | | 0.355 cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) | |
| Measurement range of flux density | | 0.1 - 10^4 neutrons $\cdot\text{s}^{-1}\cdot\text{cm}^{-2}$ | | 0.1 - 10^4 neutrons $\cdot\text{s}^{-1}\cdot\text{cm}^{-2}$ | |
| Typical sensitivity to Pu-Be radiation, (In flux density measurement mode) | | 0.5 cps/(neutrons $\cdot\text{s}^{-1}\cdot\text{cm}^{-2}$) | | 0.5 cps/(neutrons $\cdot\text{s}^{-1}\cdot\text{cm}^{-2}$) | |
| Limits of tolerable intrinsic relative error | <i>dose rate</i> <i>flux density</i> | $\pm 35\%$ $\pm 20\%$ | | $\pm 20\%$ $\pm 35\%$ | |
| Protection class | | IP64 | | IP64 | |
| Interface | | RS232 | RS485 | RS232 | RS485 |
| Operation temperature range | | -40...+50°C | | -40...+50°C | |
| Dimensions, weight | | Ø90x260 mm, 2 kg | | 316x220x265 mm, 8 kg | |
| Image | |  | |  | |

| Detection Unit | | BDKN-05 | BDKN-06 |
|--|---|---|--|
| Detector: He-3 proportional counter in polyethylene moderator | | Two He-3 counters | One He-3 counter |
| Energy range | | 0.025 eV – 14 MeV | 0.025 eV – 16 MeV |
| Measurement range of ambient dose equivalent rate | | – | 0.1 $\mu\text{Sv/h}$ – 30 mSv/h |
| Typical sensitivity to Pu-Be radiation, (In dose rate measurement mode) | | – | 0.7 cps/($\mu\text{Sv}\cdot\text{h}^{-1}$) |
| Measurement range of flux density | | 0.1 – $2\cdot 10^3$ neutrons $\cdot\text{s}^{-1}\cdot\text{cm}^{-2}$ | – |
| Typical sensitivity to Pu-Be radiation, (In flux density measurement mode) | | 10 cps/(neutrons $\cdot\text{s}^{-1}\cdot\text{cm}^{-2}$) | 1 cps/(neutrons $\cdot\text{s}^{-1}\cdot\text{cm}^{-2}$) |
| Limits of tolerable intrinsic relative error | <i>dose rate</i> <i>flux density</i> | – $\pm 20\%$ | $\pm 20\%$ – |
| Protection class | | IP54 | IP64 |
| Interface | | RS232 | RS232 |
| Operation temperature range | | -20...+50°C | -30...+50°C |
| Dimensions, weight | | 105x115x380 mm, 3.5 kg | 550x254x254 mm, 10 kg (w/o tripod) |
| Image | |  |  |

Design and specifications are subject to change without notice